


User Guide

Vaisala Indigo-compatible
humidity and temperature probes

HMP Series with MMP8 and TMP1

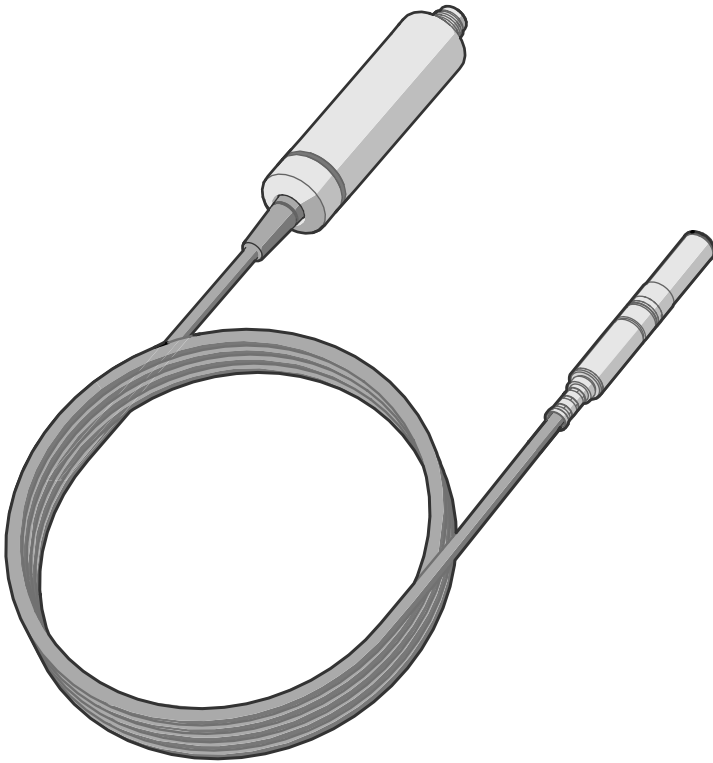

VAISALA

PUBLISHED BY

Vaisala Oyj
Vanha Nurmijärventie 21, FI-01670 Vantaa, Finland
P.O. Box 26, FI-00421 Helsinki, Finland
+358 9 8949 1
www.vaisala.com
docs.vaisala.com

© Vaisala 2024

No part of this document may be reproduced, published, or publicly displayed in any form or by any means, electronic or mechanical (including photocopying), nor may its contents be modified, translated, adapted, sold, or disclosed to a third party without prior written permission of the copyright holder. Translated documents and translated portions of multilingual documents are based on the original English versions. In ambiguous cases, the English versions are applicable, not the translations.

The contents of this document are subject to change without prior notice.

Local rules and regulations applicable to the products and services may vary and they shall take precedence over the information contained in this document. Vaisala makes no representations on this document's compliance with the local rules and regulations applicable at any

given time, and hereby disclaims any and all responsibilities related thereto. You are instructed to confirm the applicability of the local rules and regulations and their effect on the intended use of the products and services.

This document does not create any legally binding obligations for Vaisala towards customers or end users. All legally binding obligations are set forth exclusively in the applicable contract or in the relevant set of General Conditions of Vaisala (www.vaisala.com/policies).

This product contains software developed by Vaisala or third parties. Use of the software is governed by license terms and conditions included in the applicable contract or, in the absence of separate license terms and conditions, by the General License Conditions of Vaisala Group.

Table of contents

| | | |
|-----------|---|----|
| 1. | About this document | 11 |
| 1.1 | Version information..... | 11 |
| 1.2 | Related manuals..... | 14 |
| 1.3 | Documentation conventions..... | 15 |
| 1.4 | Trademarks..... | 15 |
| 2. | Product overview | 16 |
| 2.1 | Probe structure..... | 16 |
| 2.2 | Basic features and options..... | 17 |
| 2.3 | Output parameters..... | 17 |
| 2.4 | Additional features with Indigo transmitters..... | 18 |
| 2.5 | Safety..... | 19 |
| 2.6 | ESD protection..... | 19 |
| 2.7 | Regulatory statements..... | 20 |
| 2.7.1 | FCC Part 15 compliance statement..... | 20 |
| 2.7.2 | Canada ICES-3 / NMB-3 compliance statement..... | 20 |
| 3. | Functional description | 21 |
| 3.1 | HUMICAP technology..... | 21 |
| 3.2 | Sensor purge..... | 21 |
| 3.3 | Condensation prevention functions..... | 22 |
| 3.4 | Environmental compensation..... | 23 |
| 3.4.1 | Pressure compensation..... | 23 |
| 3.4.2 | Temperature compensation..... | 23 |
| 3.5 | Filtering factor..... | 24 |
| 4. | Installation | 26 |
| 4.1 | Probe holder ASM213582..... | 27 |
| 4.1.1 | Mounting the probe body using probe holder ASM213582..... | 27 |
| 4.2 | Wiring..... | 28 |
| 4.3 | HMP1 probe..... | 29 |
| 4.4 | HMP3 probe..... | 30 |
| 4.4.1 | Vapor-tight installations with cable gland..... | 31 |
| 4.4.2 | Duct installation kit for humidity probe..... | 31 |
| 4.4.3 | Probe holder ASM213382..... | 31 |
| 4.5 | HMP4 probe..... | 32 |
| 4.6 | HMP5 probe..... | 33 |
| 4.7 | HMP7 probe..... | 34 |
| 4.7.1 | Example installation of a heated probe head..... | 36 |
| 4.7.2 | Vapor-tight installations with cable gland..... | 36 |
| 4.7.3 | Duct installation kit for humidity probe..... | 37 |
| 4.7.4 | Pressure-tight Swagelok installation kit..... | 37 |
| 4.8 | HMP8 probe..... | 38 |

| | | |
|-----------|--|-----------|
| 4.9 | HMP9 probe..... | 39 |
| 4.9.1 | Installing HMP9 through a cable gland..... | 40 |
| 4.9.2 | Overview of HMP9 Duct Installation Kit..... | 41 |
| 4.9.3 | Mounting HMP9 probe head with Duct Installation Kit..... | 42 |
| 4.10 | MMP8 probe..... | 44 |
| 4.10.1 | Moisture ppm calculation for transformer oils..... | 45 |
| 4.11 | TMP1 probe..... | 46 |
| 4.11.1 | Duct installation kit for temperature probe..... | 47 |
| 4.11.2 | Pressure-tight Swagelok installation kit..... | 47 |
| 4.12 | DTR502B solar radiation shield..... | 48 |
| 4.12.1 | Mounting probe head inside DTR502B..... | 49 |
| 4.13 | Configuring environmental compensations..... | 51 |
| 5. | Configuration with Insight software..... | 53 |
| 5.1 | Vaisala Insight software..... | 53 |
| 5.2 | Connecting to Insight software..... | 53 |
| 5.3 | Configuration options..... | 54 |
| 5.4 | Configuring condensation prevention with Insight..... | 54 |
| 5.5 | Diagnostics in Insight..... | 55 |
| 6. | Using probe with Indigo transmitters..... | 57 |
| 6.1 | Connecting probe to Indigo200 series transmitters..... | 57 |
| 6.2 | Connecting probe to Indigo300 transmitter..... | 58 |
| 6.3 | Connecting probes to Indigo500 series transmitters..... | 59 |
| 6.4 | Default analog output configuration with Indigo transmitters..... | 60 |
| 7. | Using probe with Indigo80 handheld indicator..... | 62 |
| 7.1 | Indigo80 handheld indicator..... | 62 |
| 7.1.1 | Probe compatibility..... | 63 |
| 7.1.2 | Indigo80 keypad..... | 63 |
| 7.1.3 | Indigo80 main menu..... | 63 |
| 7.2 | Connecting probes to Indigo80..... | 64 |
| 7.3 | Configuring probe features with Indigo80 handheld indicator..... | 66 |
| 7.3.1 | Example of configuring filtering factor with Indigo80 handheld indicator..... | 66 |
| 7.4 | Configuring environment settings with Indigo80 handheld indicator.... | 67 |
| 7.4.1 | Example of enabling temperature compensation with Indigo80 handheld indicator (HMP7 and TMP1)..... | 69 |
| 8. | Calibration and adjustment..... | 71 |
| 8.1 | Calibration and adjustment overview..... | 71 |
| 8.2 | Adjustment points and requirements..... | 71 |
| 8.3 | HMK15 Humidity Calibrator with HMP Series probes | 72 |
| 8.4 | Adjusting measurement with Insight software..... | 74 |
| 8.5 | Adjusting measurement with Indigo transmitter..... | 75 |

| | | |
|--|---|------------|
| 8.6 | Calibration and adjustment with Indigo80 handheld indicator..... | 76 |
| 8.6.1 | Performing guided calibration with Indigo80 handheld indicator... .. | 77 |
| 8.6.2 | Performing manual adjustment with Indigo80 handheld indicator..... | 78 |
| 8.6.3 | Restoring factory adjustment with Indigo80 handheld indicator..... | 79 |
| 9. | Maintenance..... | 81 |
| 9.1 | Cleaning the HMP and TMP probes..... | 81 |
| 9.2 | Cleaning the MMP8 probe..... | 81 |
| 9.3 | Chemical tolerance..... | 82 |
| 9.4 | Changing the probe filter..... | 82 |
| 9.5 | Replacing the HUMICAP® sensor..... | 83 |
| 10. | Troubleshooting..... | 86 |
| 10.1 | Problem situations..... | 86 |
| 10.2 | Error messages..... | 87 |
| 10.3 | Restoring factory default settings with Insight software..... | 89 |
| 10.4 | Restoring factory default settings with Indigo80 handheld indicator.... | 89 |
| 11. | Technical data..... | 90 |
| 11.1 | HMP1 specifications..... | 90 |
| 11.2 | HMP3 specifications..... | 93 |
| 11.3 | HMP4 specifications..... | 97 |
| 11.4 | HMP5 specifications..... | 101 |
| 11.5 | HMP7 specifications..... | 105 |
| 11.6 | HMP8 specifications..... | 109 |
| 11.7 | HMP9 specifications..... | 114 |
| 11.8 | MMP8 specifications..... | 118 |
| 11.9 | TMP1 specifications..... | 121 |
| 11.10 | Accessories and spare parts..... | 124 |
| 11.11 | Accuracy of calculated output parameters..... | 129 |
| Appendix A: Modbus reference..... | | 131 |
| A.1 | Default communication settings..... | 131 |
| A.2 | Function codes..... | 131 |
| A.3 | Data encoding..... | 131 |
| A.3.1 | 32-bit floating point or 32-bit integer format..... | 132 |
| A.3.2 | 16-bit integer format..... | 132 |
| A.4 | Modbus registers..... | 132 |
| A.4.1 | Measurement data registers..... | 133 |
| A.4.2 | Configuration registers..... | 135 |
| A.4.3 | Status registers..... | 138 |
| A.4.4 | Test value registers..... | 140 |
| A.5 | Device identification objects..... | 140 |
| A.6 | Exception responses..... | 141 |
| A.7 | Modbus communication examples..... | 142 |
| Maintenance and calibration services..... | | 145 |

Warranty..... 145

Technical support..... 145

Recycling..... 145

List of figures

| | | |
|-----------|---|----|
| Figure 1 | Probe parts..... | 16 |
| Figure 2 | Example installation..... | 26 |
| Figure 3 | Probe holder ASM213582 dimensions..... | 27 |
| Figure 4 | M12 5-pin A-coded male connector pinout..... | 28 |
| Figure 5 | RS-485 wiring..... | 29 |
| Figure 6 | HMP1 probe dimensions..... | 29 |
| Figure 7 | HMP3 probe dimensions..... | 30 |
| Figure 8 | Probe holder ASM213382..... | 31 |
| Figure 9 | HMP4 probe dimensions..... | 32 |
| Figure 10 | HMP5 probe dimensions..... | 33 |
| Figure 11 | Optional mounting flange 210696 dimensions..... | 33 |
| Figure 12 | HMP7 probe dimensions..... | 34 |
| Figure 13 | Heated probe and temperature probe installation in a climate chamber..... | 36 |
| Figure 14 | HMP7 installation to pipeline using a Swagelok installation kit..... | 37 |
| Figure 15 | HMP8 probe dimensions..... | 38 |
| Figure 16 | HMP9 probe dimensions..... | 39 |
| Figure 17 | Installing HMP9 probe head through a cable gland..... | 40 |
| Figure 18 | Duct Installation Kit ASM214055 dimensions..... | 41 |
| Figure 19 | Duct installation overview..... | 42 |
| Figure 20 | MMP8 dimensions..... | 44 |
| Figure 21 | TMP1 probe dimensions..... | 46 |
| Figure 22 | Optional duct kit 215003 dimensions..... | 47 |
| Figure 23 | TMP1 installation to pipeline using a Swagelok installation kit..... | 48 |
| Figure 24 | DTR502B dimensions..... | 49 |
| Figure 25 | Mounting DTR502B on a pole mast..... | 50 |
| Figure 26 | HMP9 probe head with sensor head support 215130..... | 51 |
| Figure 27 | Connecting probe to Insight using Indigo USB adapter..... | 53 |
| Figure 28 | HMP5 in Insight software..... | 54 |
| Figure 29 | HMP5 diagnostics in Insight (advanced mode)..... | 56 |
| Figure 30 | Connecting probe to Indigo200 series transmitter..... | 58 |
| Figure 31 | Connecting probe to Indigo300 transmitter..... | 59 |
| Figure 32 | Connecting probes to Indigo500 transmitter..... | 60 |
| Figure 33 | Indigo80 handheld indicator..... | 62 |
| Figure 34 | Indigo80 keypad..... | 63 |
| Figure 35 | Indigo80 main menu..... | 63 |
| Figure 36 | Connecting probes to Indigo80..... | 64 |
| Figure 37 | HMP5 calibration with HMK15 using 211302SP adapter..... | 72 |
| Figure 38 | Using HMP9 calibration adapter with HMK15..... | 73 |
| Figure 39 | Indigo80 calibration methods for probes..... | 77 |
| Figure 40 | Example: HMP3 probe head with filter removed..... | 84 |
| Figure 41 | HMP1 humidity measurement accuracy as a function of temperature..... | 91 |
| Figure 42 | HMP1 temperature measurement accuracy over full range..... | 91 |
| Figure 43 | HMP1 probe dimensions..... | 93 |

| | | |
|-----------|--|-----|
| Figure 44 | HMP3 humidity measurement accuracy as a function of temperature..... | 94 |
| Figure 45 | HMP3 temperature measurement accuracy over full range..... | 94 |
| Figure 46 | HMP3 probe dimensions..... | 97 |
| Figure 47 | HMP4 humidity measurement accuracy as a function of temperature..... | 98 |
| Figure 48 | HMP4 temperature measurement accuracy over full range..... | 98 |
| Figure 49 | HMP4 probe dimensions..... | 101 |
| Figure 50 | HMP5 humidity measurement accuracy as a function of temperature..... | 102 |
| Figure 51 | HMP5 temperature measurement accuracy over full range..... | 102 |
| Figure 52 | HMP5 probe dimensions..... | 105 |
| Figure 53 | HMP7 humidity measurement accuracy as a function of temperature..... | 106 |
| Figure 54 | HMP7 temperature measurement accuracy over full range..... | 106 |
| Figure 55 | HMP7 probe dimensions..... | 109 |
| Figure 56 | HMP8 humidity measurement accuracy as a function of temperature..... | 110 |
| Figure 57 | HMP8 temperature measurement accuracy over full range..... | 110 |
| Figure 58 | HMP8 probe dimensions..... | 113 |
| Figure 59 | Optional ball valve kit dimensions..... | 114 |
| Figure 60 | HMP9 humidity measurement accuracy as a function of temperature..... | 115 |
| Figure 61 | HMP9 temperature measurement accuracy over full range..... | 116 |
| Figure 62 | HMP9 probe dimensions..... | 118 |
| Figure 63 | MMP8 A _w measurement accuracy..... | 119 |
| Figure 64 | MMP8 dimensions..... | 121 |
| Figure 65 | TMP1 temperature measurement accuracy over full range..... | 122 |
| Figure 66 | TMP1 probe dimensions..... | 124 |
| Figure 67 | Vaisala Humidity Calculator in Advanced mode..... | 130 |

List of tables

| | | |
|----------|---|-----|
| Table 1 | Document versions (English)..... | 11 |
| Table 2 | Related manuals..... | 14 |
| Table 3 | Availability of output parameters..... | 17 |
| Table 4 | Oil solubility coefficients for Vaisala moisture in oil products..... | 45 |
| Table 5 | Default analog output configuration per output parameter..... | 60 |
| Table 6 | Suitability of cleaning agents..... | 82 |
| Table 7 | Troubleshooting table..... | 86 |
| Table 8 | HMP1 measurement performance..... | 90 |
| Table 9 | HMP1 operating environment..... | 91 |
| Table 10 | HMP1 inputs and outputs..... | 92 |
| Table 11 | HMP1 output parameters..... | 92 |
| Table 12 | HMP1 compliance..... | 92 |
| Table 13 | HMP1 mechanical specifications..... | 92 |
| Table 14 | HMP3 measurement performance..... | 93 |
| Table 15 | HMP3 operating environment..... | 94 |
| Table 16 | HMP3 inputs and outputs..... | 95 |
| Table 17 | HMP3 output parameters..... | 95 |
| Table 18 | HMP3 compliance..... | 96 |
| Table 19 | HMP3 mechanical specifications..... | 96 |
| Table 20 | HMP4 measurement performance..... | 97 |
| Table 21 | HMP4 operating environment..... | 99 |
| Table 22 | HMP4 inputs and outputs..... | 99 |
| Table 23 | HMP4 output parameters..... | 99 |
| Table 24 | HMP4 compliance..... | 100 |
| Table 25 | HMP4 mechanical specifications..... | 100 |
| Table 26 | HMP5 measurement performance..... | 101 |
| Table 27 | HMP5 operating environment..... | 103 |
| Table 28 | HMP5 inputs and outputs..... | 103 |
| Table 29 | HMP5 output parameters..... | 103 |
| Table 30 | HMP5 compliance..... | 104 |
| Table 31 | HMP5 mechanical specifications..... | 104 |
| Table 32 | HMP7 measurement performance..... | 105 |
| Table 33 | HMP7 operating environment..... | 107 |
| Table 34 | HMP7 inputs and outputs..... | 107 |
| Table 35 | HMP7 output parameters..... | 107 |
| Table 36 | HMP7 compliance..... | 108 |
| Table 37 | HMP7 mechanical specifications..... | 108 |
| Table 38 | HMP8 measurement performance..... | 109 |
| Table 39 | HMP8 operating environment..... | 111 |
| Table 40 | HMP8 inputs and outputs..... | 111 |
| Table 41 | HMP8 output parameters..... | 111 |
| Table 42 | HMP8 compliance..... | 112 |
| Table 43 | HMP8 mechanical specifications..... | 112 |
| Table 44 | HMP9 measurement performance..... | 114 |
| Table 45 | HMP9 operating environment..... | 116 |

| | | |
|----------|--|-----|
| Table 46 | HMP9 inputs and outputs..... | 116 |
| Table 47 | HMP9 output parameters..... | 117 |
| Table 48 | HMP9 compliance..... | 117 |
| Table 49 | HMP9 mechanical specifications..... | 117 |
| Table 50 | MMP8 measurement performance..... | 118 |
| Table 51 | MMP8 operating environment..... | 119 |
| Table 52 | MMP8 inputs and outputs..... | 119 |
| Table 53 | MMP8 compliance..... | 120 |
| Table 54 | MMP8 mechanical specifications..... | 120 |
| Table 55 | TMP1 measurement performance..... | 121 |
| Table 56 | TMP1 operating environment..... | 122 |
| Table 57 | TMP1 inputs and outputs..... | 123 |
| Table 58 | TMP1 compliance..... | 123 |
| Table 59 | TMP1 mechanical specifications..... | 123 |
| Table 60 | Connection cables..... | 124 |
| Table 61 | HMP3 accessories..... | 125 |
| Table 62 | HMP3 spare parts..... | 125 |
| Table 63 | HMP4 spare parts..... | 126 |
| Table 64 | HMP5 accessories..... | 126 |
| Table 65 | HMP5 spare parts..... | 126 |
| Table 66 | HMP7 accessories..... | 127 |
| Table 67 | HMP7 spare parts..... | 127 |
| Table 68 | HMP8 accessories..... | 127 |
| Table 69 | HMP8 spare parts..... | 128 |
| Table 70 | HMP9 accessories..... | 128 |
| Table 71 | HMP9 spare parts..... | 128 |
| Table 72 | MMP8 accessories..... | 129 |
| Table 73 | MMP8 spare parts..... | 129 |
| Table 74 | TMP1 accessories..... | 129 |
| Table 75 | Default Modbus serial communication settings..... | 131 |
| Table 76 | Modbus function codes..... | 131 |
| Table 77 | Interpretation of 16-bit signed integer values..... | 132 |
| Table 78 | Floating point measurement data registers (read-only)..... | 133 |
| Table 79 | Integer measurement data registers (read-only)..... | 134 |
| Table 80 | Modbus configuration data registers (writable)..... | 135 |
| Table 81 | Modbus function registers (writable)..... | 138 |
| Table 82 | Modbus status data registers (read-only)..... | 138 |
| Table 83 | Error codes in register 0203 _{hex} | 139 |
| Table 84 | Modbus test registers (read-only)..... | 140 |
| Table 85 | Device identification objects..... | 140 |
| Table 86 | Modbus exception responses..... | 141 |

1. About this document

1.1 Version information

This document provides instructions for installing, using, and maintaining Vaisala HUMICAP® Humidity and Temperature Probes HMP1, HMP3, HMP4, HMP5, HMP7, HMP8, HMP9, Moisture in Oil Probe MMP8, and Temperature Probe TMP1.

Table 1 Document versions (English)

| Document code | Date | Description |
|---------------|--------------|--|
| M212022EN-K | January 2024 | <p>Applicable from software version 1.2.8 onward.</p> <p>Added information on the LED behaviour of HMP3 and HMP7 to Probe structure (page 16) and Problem situations (page 86).</p> <p>Updated the description of environmental compensation in Environmental compensation (page 23). Added information on temperature compensation using the Indigo80 handheld indicator and the Indigo520 transmitter to Temperature compensation (page 23).</p> <p>Updated instructions on configuring the environment settings in Configuring environment settings with Indigo80 handheld indicator (page 67).</p> <p>Added an example of enabling temperature compensation to Example of enabling temperature compensation with Indigo80 handheld indicator (HMP7 and TMP1) (page 69).</p> <p>Updated information on the lengths of the MMP8 probe in MMP8 probe (page 44) and MMP8 specifications (page 118). The MMP8 probe is now available in two different lengths (262 mm and 448 mm).</p> <p>Added a new accessory, weatherproof carrying case, to Accessories and spare parts (page 124) for MMP8 and HMP8. Description of DRW212076SP updated.</p> <p>Corrected the output unit of water concentration in oil to be ppm_w throughout the document.</p> <p>Added information on default analog output values to Default analog output configuration with Indigo transmitters (page 60).</p> <p>Updated the HMP8, MMP8 and TMP1 dimension drawings.</p> <p>Added information on the probe calibration reminder and interval to Calibration and adjustment overview (page 71).</p> <p>The change list continues on the next page.</p> |

| Document code | Date | Description |
|---------------|--------------|---|
| M212022EN-K | January 2024 | <p>Continued from the previous page.</p> <p>Updated the instructions on calibrating the probe with Indigo80 in:</p> <ul style="list-style-type: none"> • Performing guided calibration with Indigo80 handheld indicator (page 77) • Performing manual adjustment with Indigo80 handheld indicator (page 78) • Restoring factory adjustment with Indigo80 handheld indicator (page 79) <p>Updated instructions on restoring factory default settings with Indigo80 in Restoring factory default settings with Indigo80 handheld indicator (page 89).</p> <p>Updated the storage temperature ranges for HMP4, HMP5, HMP7, HMP8 and TMP1 probes in:</p> <ul style="list-style-type: none"> • HMP4 specifications (page 97) • HMP5 specifications (page 101) • HMP7 specifications (page 105) • HMP8 specifications (page 109) • TMP1 specifications (page 121) <p>Updated the probe cable lengths for HMP3, HMP7 and HMP8 probes in:</p> <ul style="list-style-type: none"> • HMP3 specifications (page 93) • HMP7 specifications (page 105) • HMP8 specifications (page 109) <p>Added T63 response time for the HMP1 probe in HMP1 specifications (page 90).</p> |

| Document code | Date | Description |
|---------------|-----------|---|
| M212022EN-J | June 2023 | <p>Applicable from software version 1.2.8 onward.</p> <p>Updated information on external temperature sources in Environmental compensation (page 23).</p> <p>Added information on a magnetic probe holder accessory to Probe holder ASM213382 (page 31) and Accessories and spare parts (page 124) for HMP3 and HMP7.</p> <p>Added information on Moisture ppm calculation for transformer oils (page 45) for MMP8.</p> <p>Added information on the Indigo300 transmitter and updated information on other Indigo transmitters in:</p> <ul style="list-style-type: none"> • Additional features with Indigo transmitters (page 18) • Using probe with Indigo transmitters (page 57) • Adjusting measurement with Indigo transmitter (page 75) <p>Updated instruction Replacing the HUMICAP® sensor (page 83).</p> <p>Added information on max. T_d temperatures to specifications of the following probes: HMP3, HMP4, HMP5, HMP6, HMP7, HMP8 and HMP9.</p> <p>Updated information on connection cables in Accessories and spare parts (page 124). Updated accessories and spare parts information for the following probes: HMP3, HMP4, HMP5, HMP7, HMP8, HMP9 and MMP8.</p> |

| Document code | Date | Description |
|---------------|------------|--|
| M212022EN-H | March 2023 | <p>Added information on the Indigo80 handheld indicator, environmental compensation, filtering factor, and accuracy of calculated output parameters. Added sections:</p> <ul style="list-style-type: none"> • Environmental compensation (page 23) • Filtering factor (page 24) • Configuring environmental compensations (page 51) • Using probe with Indigo80 handheld indicator • Calibration and adjustment with Indigo80 handheld indicator (page 76) • Restoring factory default settings with Indigo80 handheld indicator (page 89) • Accuracy of calculated output parameters (page 129) <p>Updated sections:</p> <ul style="list-style-type: none"> • Product overview (page 16) • Basic features and options (page 17) • Calibration and adjustment overview (page 71) • Accessories and spare parts (page 124) <p>In section <i>Installation</i>, added information on optional installation kits available for the following probes: HMP3, HMP7, and TMP1. Updated information on the fuel cell application for HMP7 and ball valve for HMP8 and MMP8. Deleted section <i>Attaching ball valve kit to process</i>.</p> <p>Indigo200 series transmitters and Adjusting measurement with Indigo transmitter (page 75) revised to describe the current Indigo200 transmitters compatible with the Insight PC software.</p> <p>Section <i>Calibration and adjustment</i> separated from <i>Maintenance</i>.</p> |

1.2 Related manuals



For the latest versions of these documents, see docs.vaisala.com.

Table 2 Related manuals

| Document code | Name |
|---------------|--|
| M211982EN | Vaisala HMP Series with MMP8 and TMP1 Quick Guide |
| M212842EN | Vaisala Indigo201 Analog Output Transmitter User Guide |
| M212843EN | Vaisala Indigo202 Digital Transmitter User Guide |

| Document code | Name |
|---------------|--|
| M212287EN | Vaisala Indigo500 Series Transmitters User Guide |
| M212722EN | Vaisala Indigo80 Handheld Indicator User Guide |

1.3 Documentation conventions



WARNING! Warning alerts you to a serious hazard. If you do not read and follow instructions carefully at this point, there is a risk of injury or even death.



CAUTION! Caution warns you of a potential hazard. If you do not read and follow instructions carefully at this point, the product could be damaged or important data could be lost.



Highlights important information on using the product.



Gives information for using the product more efficiently.



Lists tools needed to perform the task.



Indicates that you need to take some notes during the task.

1.4 Trademarks

Vaisala® and HUMICAP® are registered trademarks of Vaisala Oyj.

Modbus® is a registered trademark of Schneider Automation Inc.

All other product or company names that may be mentioned in this publication are trade names, trademarks, or registered trademarks of their respective owners.

2. Product overview

HMP series probes are humidity and temperature measurement probes with a digital output (Modbus® protocol). The probes are designed for demanding humidity and temperature measurement applications. The probes have a two-part structure, with measurement electronics contained in the probe body and sensor(s) in the probe head. The probe body and the probe head are connected by a fixed cable, except on the HMP1 model. Length options for this connecting cable depend on the probe model.

The probes are compatible with Vaisala Indigo transmitters and Vaisala Indigo80 Handheld Indicator. They can also be connected to Vaisala Insight software for configuration, calibration, adjustment, diagnostics, and temporary online monitoring.

2.1 Probe structure

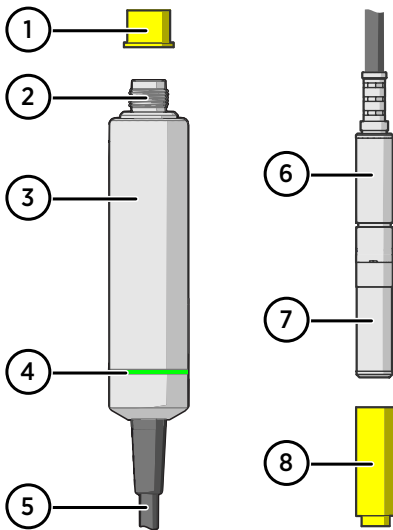


Figure 1 Probe parts

- 1 Protection cap (remove before use)
- 2 5-pin M12 connector
- 3 Probe body with type label
- 4 Status indicator LED:
 - Green Power on and probe online, flashes when communicating
 - Red Error
 - Off Power off, or indicator disabled
- 5 Fixed probe cable, variable length (do not cut).
HMP1 model does not have a probe cable, as its probe head is directly attached to the probe body.
- 6 Probe head (HMP7 model shown)
- 7 Location of sensor(s) on the probe head. Other probe models have a removable filter over the sensors but HMP1, HMP9, and TMP1 do not.
- 8 Protection cap (remove before use)



To prevent the warming of the indicator LED from causing a slight measurement error, HMP1 keeps the indicator normally off (even when power is on). The same applies to HMP3 and HMP7 probes that have a 0.15-m (0.49-ft) probe connection cable. If the probe is in error state, the red LED is shown.

2.2 Basic features and options

- Comprehensive list of output parameters
- Sensor purge provides superior chemical resistance (HMP models only)
- Condensation prevention feature minimizes condensation on probe (HMP models with composite sensors only)
- Traceable calibration certificate:
 - HMP and MMP models: 6 points for humidity, 1 point for temperature
 - TMP1: 2 points for temperature
- Standalone Modbus® RTU over RS-485
- Compatible with Indigo transmitters and Indigo80 handheld indicator
- Can be connected to Vaisala Insight PC software for configuration, calibration, adjustment, diagnostics, and temporary online monitoring

2.3 Output parameters



On HMP probe models, the values of all available output parameters are locked when the sensor is being warmed by the sensor purge or condensation prevention functions.

- Output parameter is available on this model.
- Output parameter is available on this model, but its value is unavailable when condensation prevention functions are warming the sensor. Writing temperature to Modbus register 0334_{hex} from an external source makes the output value available during condensation prevention.
- Output parameter is not available on this model.

Table 3 Availability of output parameters

| Output parameter | Output unit | HMP1, 3, 4, 5, 7, 8, and 9 | MMP8 | TMP1 |
|--------------------------------------|------------------|----------------------------|------|------|
| Absolute humidity | g/m ³ | ○ | – | – |
| Absolute humidity at NTP | g/m ³ | ○ | – | – |
| Dew/frost point temperature | °C | ● | – | – |
| Dew/frost point temperature at 1 atm | °C | ● | – | – |
| Dew point temperature | °C | ● | – | – |
| Dew point temperature at 1 atm | °C | ● | – | – |
| Dew point temperature difference | °C | ○ | – | – |
| Enthalpy | kJ/kg | ○ | – | – |
| Mixing ratio | g/kg | ● | – | – |
| Relative humidity | %RH | ○ | – | – |

| Output parameter | Output unit | HMP1, 3, 4, 5, 7, 8, and 9 | MMP8 | TMP1 |
|---------------------------------|------------------|-------------------------------|------|------|
| Relative humidity (dew/frost) | %RH | ● | — | — |
| Relative saturation | %RS | — | ● | — |
| Temperature | °C | ● | ● | ● |
| Water activity | - | — | ● | — |
| Water concentration | ppm _v | ● | — | — |
| Water concentration in oil | ppm _w | — | ● | — |
| Water concentration (wet basis) | vol-% | ● | — | — |
| Water mass fraction | ppm _w | ● | — | — |
| Wet-bulb temperature | °C | ● | — | — |
| Water vapor pressure | hPa | ● | — | — |
| Water vapor saturation pressure | hPa | ● | — | ● |

2.4 Additional features with Indigo transmitters

Connecting the probe to an Indigo transmitter provides a wide range of additional options for outputs, measurement viewing, status monitoring, and configuration interface access.

Examples of additional features available with Indigo520 transmitters:

- Touchscreen display for real-time data viewing and configuration
- Support for 2 probes simultaneously
- 4 configurable analog outputs
- 2 configurable relays
- 2-wire current loop analog input
- Barometer module for barometric pressure measurement (optional module)
- Ethernet connection with web interface for remote access
- Modbus TCP/IP protocol
- Service port for connecting to Indigo80 handheld indicator

Examples of additional features available with Indigo300 transmitters:

- Numerical and graphical display for real-time data viewing
- 3 pre-configurable analog outputs
- Service port on the front for connecting to Vaisala Insight PC software or Indigo80 handheld indicator for easy configuration access

Examples of additional features available with Indigo200 series transmitters:

- 3.5" TFT LCD color display or non-display model with LED indicator
- Digital output or 3 analog outputs (depending on the transmitter model)
- 2 configurable relays
- USB-C connection to Vaisala Insight PC software for easy configuration access



Available features vary depending on the Indigo transmitter model. For more information on Indigo transmitters, see www.vaisala.com/indigo.

More information

- [Default analog output configuration with Indigo transmitters \(page 60\)](#)

2.5 Safety



WARNING! When returning a product for calibration or repair, make sure it has not been exposed to dangerous contamination, and is safe to handle without special precautions.



CAUTION! Do not attempt to open the probe body. There are no user serviceable parts inside the probe body.



CAUTION! Do not touch the probe head with your bare hands. Touching will deposit impurities on the probe head.



CAUTION! Be aware that the probe head may become hot to touch when condensation prevention heating or sensor purge functions are active.

2.6 ESD protection

Electrostatic discharge (ESD) can cause immediate or latent damage to electronic circuits. Vaisala products are adequately protected against ESD for their intended use. However, it is possible to damage the product by delivering an electrostatic discharge when touching, removing or inserting any objects inside the equipment housing.

Avoid touching component contacts or connectors when working with the device.

2.7 Regulatory statements

2.7.1 FCC Part 15 compliance statement

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to Part 15 of the FCC rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that the interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.



CAUTION! Changes or modifications to this equipment not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.



This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

2.7.2 Canada ICES-3 / NMB-3 compliance statement

This Class B digital apparatus complies with Canadian ICES-003.

Cet appareil numérique de la classe B est conforme à la norme NMB-003 du Canada.

3. Functional description

3.1 HUMICAP technology

Vaisala HUMICAP® is a capacitive thin-film polymer sensor consisting of a substrate on which a thin film of polymer is deposited between two conductive electrodes. The sensing surface is coated with a porous metal electrode to protect it from contamination and exposure to condensation. The substrate is typically glass or ceramic.

The thin-film polymer either absorbs or releases water vapor as the relative humidity of the measurement environment rises or falls. The dielectric properties of the polymer film depend on the amount of absorbed water. As the relative humidity around the sensor changes, the dielectric properties of the polymer film change, and so does the capacitance of the sensor. Capacitance is converted into a humidity reading. The HUMICAP sensor is complemented by a temperature sensor, which is bonded together with the capacitive polymer on some of the sensor variants. Additional output parameters such as dew point are calculated from the readings measured by the sensors.

HUMICAP sensors with bonded temperature sensors are also known as **composite sensors**. Probes with composite sensors can use the **sensor purge** function to maintain sensor performance. They also implement **condensation prevention** functions that are a key element in achieving an excellent stability and good condensation resistance in high humidity applications.

The integrated sensor arrangement on the HMP1 and HMP9 probes is different from the composite sensors used in the other HMP probes. However, they are also capable of using condensation prevention heating and sensor purge.

3.2 Sensor purge

Sensor purge heats the sensor to a high temperature, which evaporates excess molecules out of the sensor polymer. This minimizes the drift at the wet end of humidity readings, and removes contaminants from the sensor element. The heating phase is followed by a cooling phase where the sensor cools down to ambient temperature.

During sensor purge the values of the output parameters stay frozen at their last measured values. Sensor purge takes a few minutes to complete, after which measurement continues normally and updated values of output parameters are again available.

When ordered with sensor purge enabled, HMP model probes perform the purge at one day intervals (known as **interval purge**). If desired, sensor purge can also be performed when the probe is powered on (known as **startup purge**). Purge settings can be configured with the Insight software, the Indigo80 handheld indicator, or using the Modbus protocol.



To allow the sensor purge to be completed in a reasonable time, it will not be started if the ambient temperature is below 0 °C (+32 °F).

3.3 Condensation prevention functions

Condensation prevention functions prevent water from condensing on the sensor and interfering with humidity measurement. Use of condensation prevention is controlled by a single setting that can be changed with the Insight software, the Indigo80 handheld indicator, or using the Modbus protocol. The setting is only available if your probe supports condensation prevention.

By default, condensation prevention is off.

However, the HMP7 model can be ordered from Vaisala with the feature enabled.

When condensation prevention is enabled, the probe will automatically use its available condensation prevention functions. When warming is active, values of output parameters that depend on temperature measurement (for example, relative humidity) are unavailable, unless the temperature compensation setting is set to read the temperature from an external source. Output parameters that can be measured or calculated without this external temperature information, such as dew point temperature, are available even without the temperature input.

Sensor warming

Sensor warming is available to all HMP series probes with composite sensors, HMP1, and HMP9.

Sensor warming warms the humidity sensor when necessary to keep its temperature above the dew point of the measurement environment. When sensor warming is activated, all temperature-dependent output parameters become unavailable, unless the temperature compensation setting is set to read the temperature from an external source. The output parameters become available again 4 minutes after the warming is stopped.



Sensor warming is intended for improving the condensation tolerance of the probe in measurement environments that may occasionally cause condensation to form. It is not intended for environments where continuous warming is needed.

Probe heating

Probe heating is available on HMP7 model only. Probe heating warms up the entire probe head instead of just the sensor. It is intended for use in challenging measurement environments where condensation on the probe would otherwise present a problem.

Probe heating always applies some heating power even when the sensor is not near condensation, so temperature-dependent output parameters are permanently unavailable when probe heating is used, unless external temperature information is provided to the probe.

If the ambient dew point rises close to current sensor temperature, the heating power is increased to avoid condensation.



If you use probe heating, be sure to mount the HMP7 probe head in a way that prevents the heat from being conducted away from the probe. Tightly connecting the HMP7 probe head to a metal structure may prevent the probe from maintaining probe temperature above the dew point. It will also heat the structure which may be undesirable.



Even if condensation prevention has been turned on, probe heating is not active if supply voltage is below 18 V DC. For example, this is the case when HMP7 probe is connected to Insight software using the Indigo USB Adapter.

More information

- [Configuring condensation prevention with Insight \(page 54\)](#)

3.4 Environmental compensation

Environmental compensations – pressure compensation and temperature compensation – improve the measurement accuracy of the probe. You can configure the settings with the Insight software or the Indigo80 handheld indicator, or using the Modbus protocol.

3.4.1 Pressure compensation

The pressure of the measured environment affects the accuracy of humidity calculations, especially calculations that are dependent on pressure (for example, mixing ratio). To achieve accurate output of all humidity parameters, you are recommended to update the value of the pressure compensation setpoint to match the environmental pressure when installing the probe.

For example, when you install the probe in a process with a pressure differing from normal atmospheric pressure, update the correct pressure into the pressure compensation setpoint parameter or register of the probe using the Insight software or the Indigo80 handheld indicator.

The entered value is persistent and remains unchanged at device restart.

3.4.2 Temperature compensation

Condensation prevention functions disable the probe's own temperature measurement and output parameters that depend on it. To enable temperature-dependent output parameters even when condensation prevention functions are used, you need to set an external source for the temperature compensation setpoint.

To get the most accurate measurement values, the external source needs to be able to provide the temperature compensation setpoint value constantly in real time, and the value needs to correspond to the temperature of the probe's measurement environment as accurately as possible. A suitable measurement point is as close to the probe as possible, but yet far enough so that ongoing condensation prevention warming of the probe does not have an effect on the measured value.

Temperature compensation using Indigo80 handheld indicator

If you are using the Indigo80 handheld indicator with your probe, the external temperature source can be any Indigo-compatible probe with a temperature output (for example, TMP1) that is connected to the same Indigo80 as your probe (for example, HMP7). When Indigo80 detects the connected probes, it guides you to check the probes' environment settings, where you can select to start as well as stop reading the temperature value from another probe.

When you disconnect and then reconnect the same probes to the same ports in Indigo80, Indigo80 will continue reading the temperature value from the previously selected probe. The same applies also when you restart Indigo80 with the same probes connected.

Temperature compensation using Indigo520 transmitter

If you are using the Indigo520 transmitter with your probes, TMP1 can function as the temperature source for HMP7. Temperature compensation turns on automatically when you connect HMP7 to probe 1 connection terminal and TMP1 to probe 2 connection terminal of the transmitter. Other probe combinations are not supported directly, but you can still update the temperature value through the Modbus TCP/IP interface of Indigo520.

For more information, see [Indigo500 User Guide \(M212287EN\)](#).

More information

- [Configuring environment settings with Indigo80 handheld indicator \(page 67\)](#)
- [Example of enabling temperature compensation with Indigo80 handheld indicator \(HMP7 and TMP1\) \(page 69\)](#)

3.5 Filtering factor

The filtering factor determines how quickly the results of measurement cycles are reflected in values of output parameters. You can use the filtering factor to slow down the response time of the measurement, filtering out rapid changes and measurement noise.

- Maximum value (1) = No filtering, fastest measurement. Output shows 100 % of the most recent measured value.
- Less than maximum value = Filtering is applied and measurement response time is reduced. For example, defining a value that is 90 % of the maximum value means that the filtered output reading = 90 % of the most recent measured value + 10 % of the previous reading.

Filtering factor settings can be configured with the Insight software, the Indigo80 handheld indicator, or using the Modbus protocol.

More information

- [Example of configuring filtering factor with Indigo80 handheld indicator \(page 66\)](#)

4. Installation

When you choose the installation location for the probe, consider the following:

- Verify the operating environment specification of the probe model. The probe head typically has a much wider operating temperature range than the probe body.
- If the temperature of the measured environment differs greatly from ambient temperature, the entire probe head and preferably plenty of cable must be inside the measured environment. This prevents measurement inaccuracy caused by heat conduction along the cable.
- Probe mounting options are model-specific.

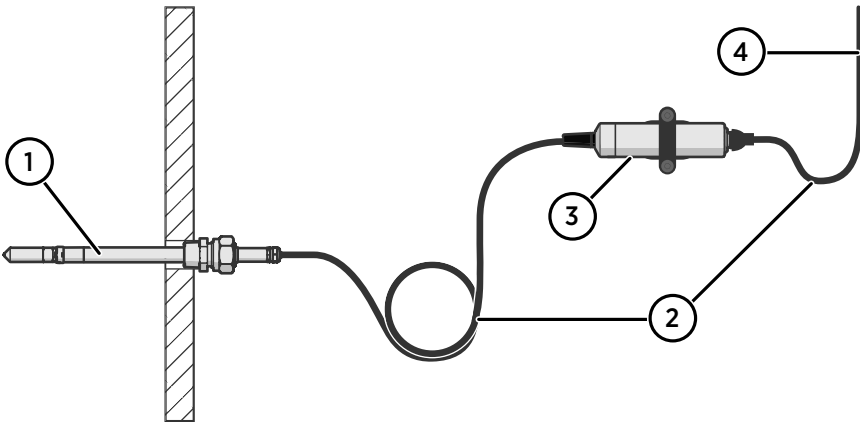



Figure 2 Example installation

- 1 Mount the probe head horizontally to prevent any water condensing on the probe head from running to the sensors.
- 2 Let the cable hang loosely to prevent condensed water from running along the cable to the probe body or probe head.
- 3 Attach the probe body to a wall or other surface using supplied probe holder (item code ASM213582).
- 4 Cable to Modbus master or Indigo device.

More information

- [Default communication settings \(page 131\)](#)

4.1 Probe holder ASM213582

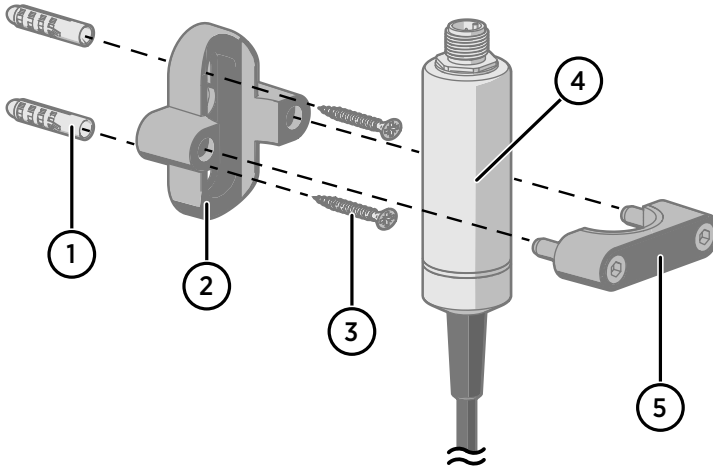

- 1 Wall plugs (2 pcs included, 6×30 nylon)
- 2 Base of the probe holder
- 3 Screws (2 pcs included, 4.8×25 DIN7981C PZ A4)
- 4 Ø 25 mm (0.98 in) probe body
- 5 Top of the probe holder with 2 hex screws (4-mm socket)

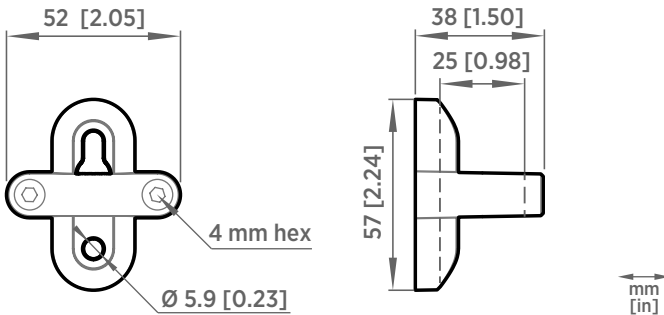


Figure 3 Probe holder ASM213582 dimensions

4.1.1 Mounting the probe body using probe holder ASM213582

Probe holder ASM213582 is designed for attaching a 25 mm probe body to a wall or other surface with screws.

- ▶ 1. Use a 4-mm Allen key to open the hex screws and remove the top part of the probe holder.
- 2. Hold the base part against the mounting surface and mark the locations of the 2 screw holes.
- 3. Drill holes at the marked locations using a 6-mm drill bit. Make the holes at least 30 mm deep.
- 4. Insert the wall plugs in the holes.
- 5. Mount the base part using screws.
- 6. Insert the probe body in the holder.
- 7. Place the top part on the base and tighten the hex screws with a 4-mm Allen key.

4.2 Wiring




Figure 4 M12 5-pin A-coded male connector pinout

| Pin # | Function | Notes | Wire colors in Vaisala cables |
|-------|-----------------------------|--|-------------------------------|
| 1 | Power supply | Operating voltage: <ul style="list-style-type: none"> • HMP7: 18–30 V DC • Other models: 15–30 V DC Current consumption: 10 mA typical, 500 mA max. | Brown |
| 2 | RS-485 - | | White |
| 3 | Power GND and RS-485 common | | Blue |
| 4 | RS-485 + | | Black |
| 5 | Not connected | | Gray |

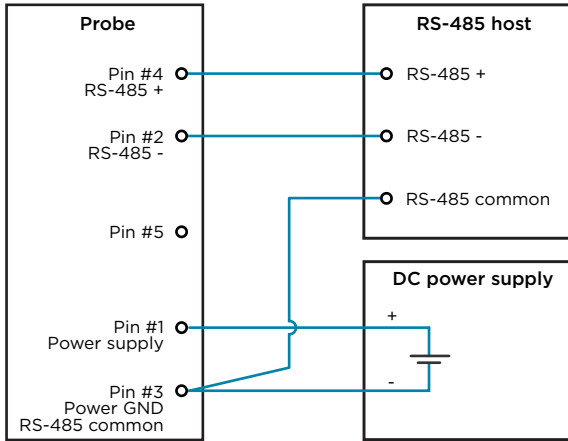


Figure 5 RS-485 wiring



Recommended maximum length of the RS-485 line is 30 m (98 ft).

4.3 HMP1 probe

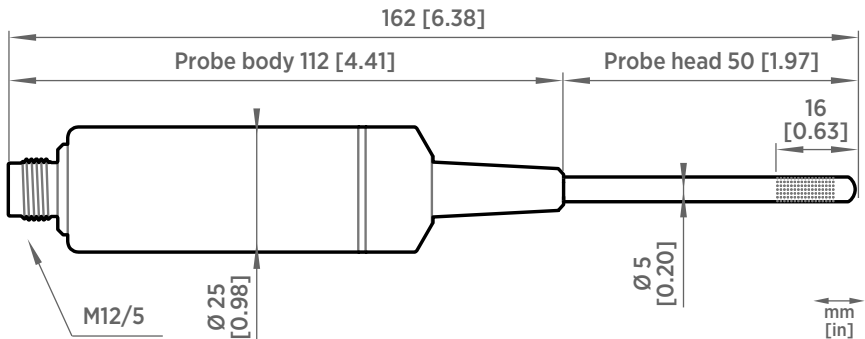


Figure 6 HMP1 probe dimensions

Vaisala HUMICAP® Humidity and Temperature Probe HMP1 is designed for ambient measurement in indoor spaces. Its probe head and body are integrated into a single unit with no cable between them. HMP1 can be directly connected to Indigo200 series transmitters to form a single wall-mounted unit.

- Operating temperature $-40 \dots +60 \text{ }^{\circ}\text{C}$ ($-40 \dots +140 \text{ }^{\circ}\text{F}$)

If purchased with a composite sensor instead of the field-replaceable HUMICAP® R2 sensor, HMP3 can use the sensor purge feature. In environments with high concentrations of chemicals and cleaning agents, sensor purge helps to maintain measurement accuracy between calibration intervals.

More information

- [Replacing the HUMICAP® sensor \(page 83\)](#)
- [Mounting probe head inside DTR502B \(page 49\)](#)

4.4.1 Vapor-tight installations with cable gland

With an AGRO M20×1.5 cable gland (Vaisala item HMP247CG), the probe cable can be installed vapor tight. For an installation example, see [Example installation of a heated probe head \(page 36\)](#).

4.4.2 Duct installation kit for humidity probe

With an optional duct installation kit (Vaisala item 210697) to support the probe head, the probe can be installed to a chamber or duct. For more information, see [Duct Installation Kit \(210697\) Installation Guide \(M212351EN\)](#).

4.4.3 Probe holder ASM213382

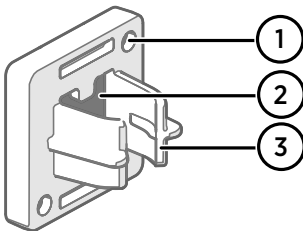


Figure 8 Probe holder ASM213382

- 1 Holes for attaching the holder with screws (screws not included)
- 2 Magnet
- 3 Probe attachment

The probe holder (Vaisala item ASM213382SP, includes 5 probe holders) is a versatile mounting accessory for securing HMP3 and HMP7 probes with a max. 2 m cable between the probe body and the probe head. To attach the probe, simply press the probe head into the probe attachment.



- The magnet can hold the weight of a max. 2 m cable between the probe body and the probe head. Do not use the magnet with probes which have probe cables longer than 2 m.
- The probe holder is not suitable for use at extreme temperatures.

Make sure that vibration or other external factors will not unintentionally change the probe position after installation. For permanent installations, Vaisala recommends attaching the holder with additional screws.

4.5 HMP4 probe

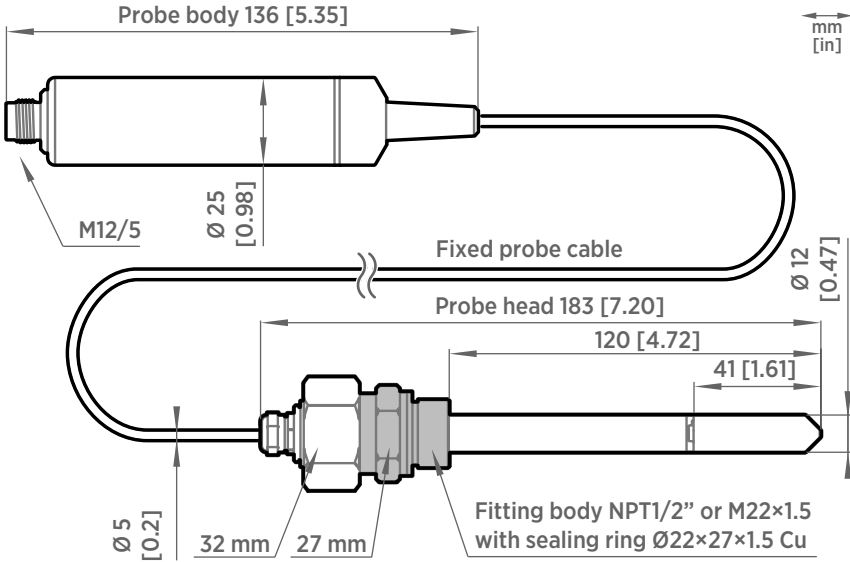


Figure 9 HMP4 probe dimensions

Vaisala HUMICAP® Humidity and Temperature Probe HMP4 is designed for high-pressure applications such as compressed air systems in maritime, breathing air, and industrial applications, where measurement performance and chemical tolerance are essential.

- Temperature measurement range -70 ... +180 °C (-94 ... +356 °F)
- Operating pressure 0-100 bar
- Operating temperature for probe body -40 ... +80 °C (-40 ... +176 °F)
- M22×1.5 or NPT1/2" fitting body



Use a sealing ring (Ø22×27×1.5 Cu) with the M22×1.5 fitting. Replace the sealing ring every time the probe is detached. Three sealing rings are supplied with the fitting.

4.6 HMP5 probe

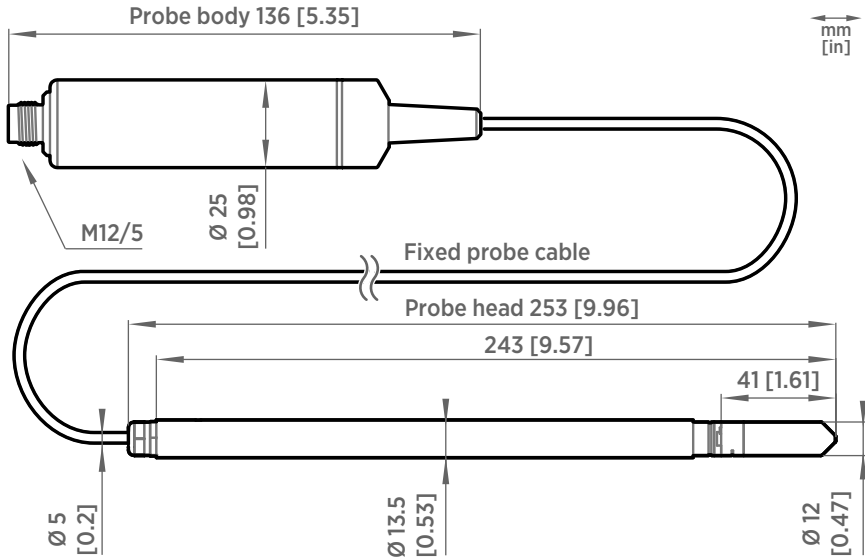


Figure 10 HMP5 probe dimensions

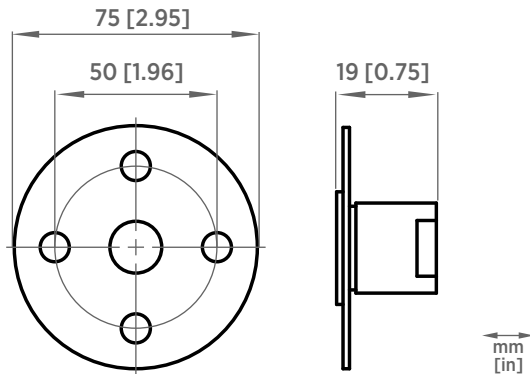


Figure 11 Optional mounting flange 210696 dimensions

Vaisala HUMICAP® Humidity and Temperature Probe HMP5 is designed for high-temperature applications such as baking ovens, pasta dryers, and industrial drying kilns, where measurement performance and chemical tolerance are essential.

- Temperature measurement range $-70 \dots +180 \text{ }^{\circ}\text{C}$ ($-94 \dots +356 \text{ }^{\circ}\text{F}$)

- Operating temperature of probe body $-40 \dots +80 \text{ }^{\circ}\text{C}$ ($-40 \dots +176 \text{ }^{\circ}\text{F}$)
- 250-mm (9.84 in) probe allows easy process installation through insulation

4.7 HMP7 probe

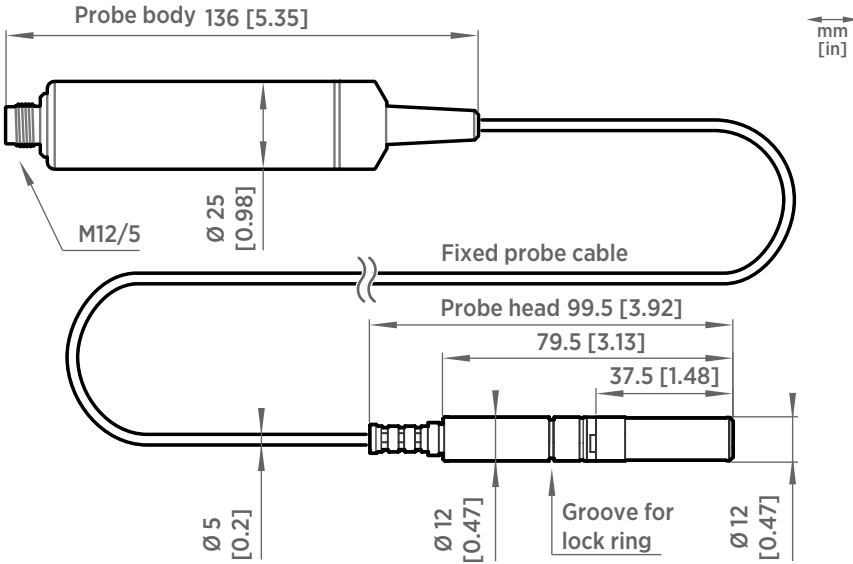


Figure 12 HMP7 probe dimensions

Vaisala HUMICAP® Humidity and Temperature Probe HMP7 is designed for applications that involve constant high humidity or rapid changes in humidity, such as drying and test chambers, combustion air, and other humidifiers and meteorological measurements, where measurement performance and chemical tolerance are essential.

- Temperature measurement range $-70 \dots +180 \text{ }^{\circ}\text{C}$ ($-94 \dots +356 \text{ }^{\circ}\text{F}$)
- Operating temperature of probe body $-40 \dots +80 \text{ }^{\circ}\text{C}$ ($-40 \dots +176 \text{ }^{\circ}\text{F}$)
- Condensation prevention with probe heating
- Vapor and pressure proof construction

Condensation prevention with probe heating

Condensation prevention on HMP7 uses a combination of probe heating and sensor warming. Probe heating keeps the entire probe head above the current dew point temperature, which prevents condensation from forming on the probe.

The values of output parameters that are dependent on temperature measurement (such as relative humidity) are unavailable when the probe is warming itself, unless the true temperature of the measured environment is updated to the temperature compensation register of the probe from another measurement instrument (for example, TMP1 model probe). Output parameters that can be measured or calculated without this external temperature information, such as dew point temperature, are available even without the temperature input.

The Indigo80 handheld indicator and Indigo500 transmitters support HMP7 temperature compensation from TMP1. For more information, see:

- [Temperature compensation \(page 23\)](#)
- [Indigo500 User Guide \(M212287EN\)](#)

HMP7 in fuel cell applications

Probe heating makes HMP7 ideal for use in fuel cell applications, specifically proton-exchange membrane fuel cells (PEMFC). Humidity measurements in fuel cell applications are performed in a high-humidity environment, typically over 80% relative humidity. Performing humidity measurements in hot, near-condensing environments is a challenging task, and the humidity sensor must be adequately protected against saturation to allow continuous measurement. Probe heating accomplishes just that.

HMP7 can be ordered from Vaisala with special settings that have been optimized for the fuel cell application. These settings include a faster probe heating control that allows the probe to quickly heat the probe to stay ahead of the rising dew point temperature.



WARNING! HMP7 is not designed for use in hazardous environments with potentially explosive atmospheres. Make sure no part of the probe is placed in a potentially explosive gas mixture.

For more information on HMP7 in fuel cell applications, see [HMP7 and HMT317/337 for Fuel Cell Applications Technical Note \(M212840EN\)](#).

More information

- [Mounting probe head inside DTR502B \(page 49\)](#)

4.7.1 Example installation of a heated probe head

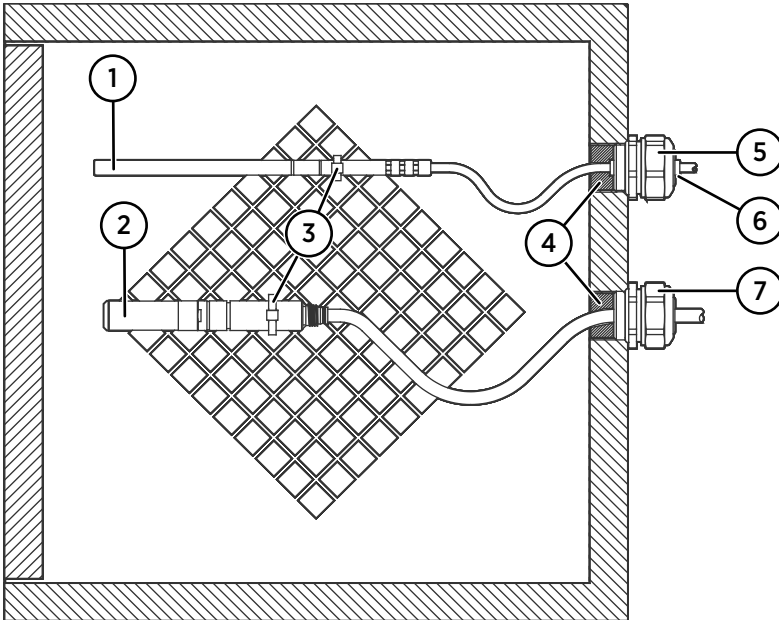


Figure 13 Heated probe and temperature probe installation in a climate chamber

- 1 Temperature probe head
- 2 Humidity probe head with probe heating
- 3 Stainless steel cable tie or similar fastener
- 4 To be sealed, for example with silicone
- 5 Cable gland, for example: AGRO 1100.12.91.065
- 6 PTFE sleeve
- 7 Cable gland AGRO (Vaisala item code HMP247CG)



Let the probe cable hang loosely to prevent condensed water from running to the probe head. Avoid attaching the heated probe head in a way that conducts the heat away, as this may prevent the probe head from maintaining a temperature that is above dew point.

4.7.2 Vapor-tight installations with cable gland

With an AGRO M20×1.5 cable gland (Vaisala item HMP247CG), the probe cable can be installed vapor tight. For an installation example, see [Example installation of a heated probe head](#) (page 36).

4.7.3 Duct installation kit for humidity probe

With an optional duct installation kit (Vaisala item 210697) to support the probe head, the probe can be installed to a chamber or duct. For more information, see [Duct Installation Kit \(210697\) Installation Guide \(M212351EN\)](#).

4.7.4 Pressure-tight Swagelok installation kit

Swagelok installation kit (Vaisala items SWG12ISO12, SWG12ISO38, and SWG12NPT12) is an optional accessory which includes a pressure-tight Swagelok® connector with ISO1/2", ISO3/8" or NPT1/2" thread.

For instructions on how to tighten the Swagelok connector properly, see the installation instructions provided with the installation kit, [SWG12ISO12 Swagelok® Connector Assembly Drawing \(DRW218087\)](#).



CAUTION! Note that overtightening the connector may damage the probe head.

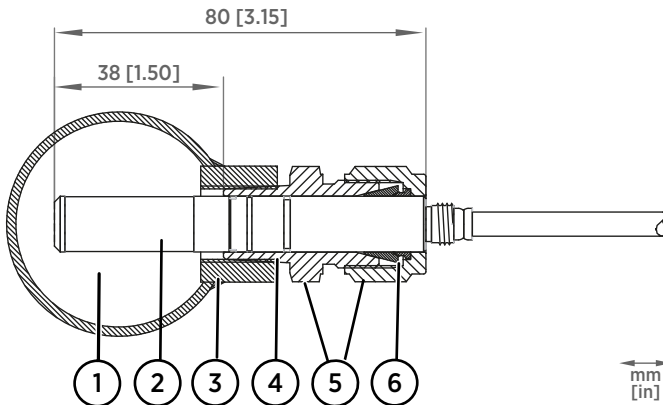


Figure 14 HMP7 installation to pipeline using a Swagelok installation kit

- 1 Max. process pressure 10 bar (145 psi), max temperature +180 °C (+356 °F)
- 2 Probe head
- 3 Duct connector
- 4 ISO1/2", ISO3/8" or NPT1/2" thread
- 5 Swagelok connector
- 6 Ferrules

4.8 HMP8 probe

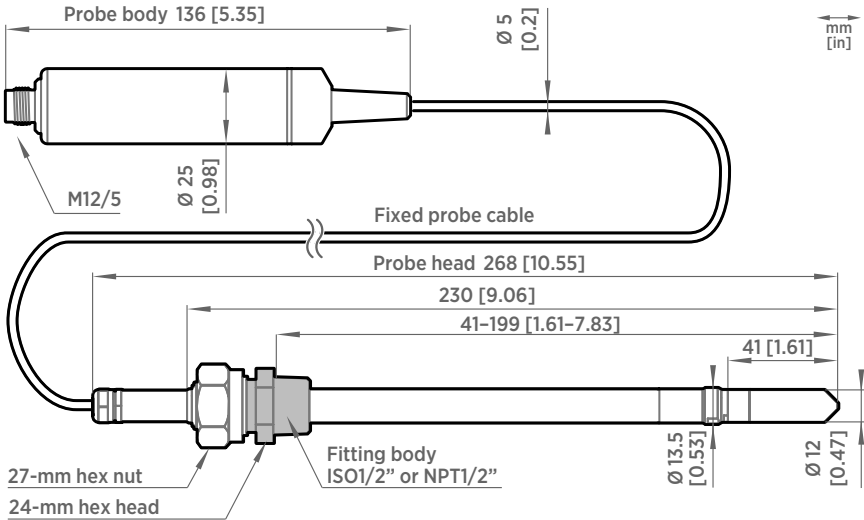


Figure 15 HMP8 probe dimensions

Vaisala HUMICAP® Humidity and Temperature Probe HMP8 is designed for pressurized applications in compressed air systems, refrigerant dryers, and other pressurized industrial applications, where easy insertion and removal of the probe and adjustable installation depth into the pipeline are needed.

- Temperature measurement range -70 ... +180 °C (-94 ... +356 °F)
- Operating temperature of probe body -40 ... +80 °C (-40 ... +176 °F)
- Operating pressure 0-40 bar
- Probe installation depth can be freely adjusted and probe can be hot-swapped from pressurized pipelines with an optional ball valve kit
- ISO1/2" or NPT1/2" fitting body

For more information on using the probe with the ball valve, see [Ball Valve Kit \(BALLVALVE-1\) Installation Guide \(M212837EN\)](#).

4.9 HMP9 probe

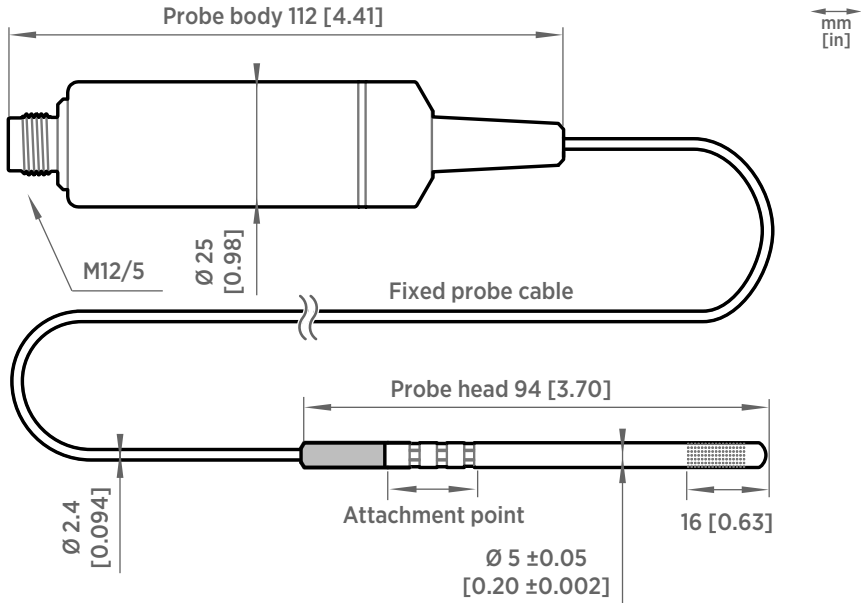


Figure 16 HMP9 probe dimensions

Vaisala HUMICAP® Humidity and Temperature Probe HMP9 is designed for easy installation into rapidly changing environments where fast response time, measurement performance, and chemical tolerance are essential.

The probe head can be mounted through thin metal walls using the included cable gland or mounting grommet. Two grommets are included: small one for 6.5 mm diameter hole, and large one for 12.5 mm diameter hole.

You can also attach the probe head directly using a zip tie. The probe head should be attached from the point near the black plastic part.

- Temperature measurement range $-40 \dots +120 \text{ }^{\circ}\text{C}$ ($-40 \dots +248 \text{ }^{\circ}\text{F}$)
- Operating temperature of probe body $-40 \dots +60 \text{ }^{\circ}\text{C}$ ($-40 \dots +140 \text{ }^{\circ}\text{F}$)
- Integrated filter (non-replaceable)



CAUTION! Do not damage the probe head by bending, crushing, or striking it. Avoid overtightening when installing the probe head through a cable gland.

More information

- [Mounting probe head inside DTR502B \(page 49\)](#)

4.9.1 Installing HMP9 through a cable gland

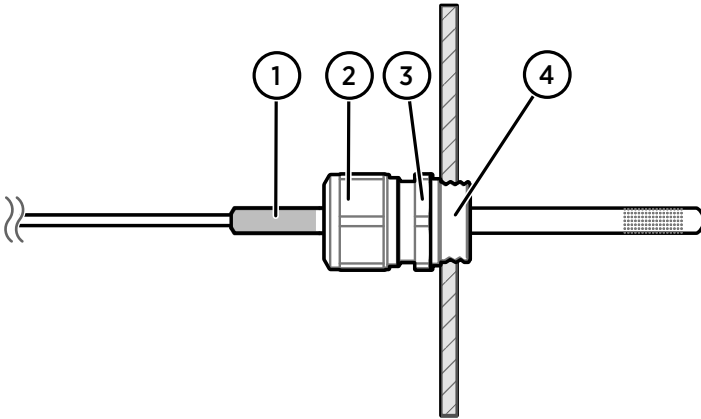


Figure 17 Installing HMP9 probe head through a cable gland

- 1 Black plastic part of the HMP9 probe head
- 2 Nut for tightening the probe in place
- 3 Base of the cable gland
- 4 M10×1.5 threads of the cable gland



- M10×1.5 cable gland (included with HMP9 probe)
- Drill with 8.5 mm bit
- M10×1.5 threading tap
- 13 mm wrench

- ▶ 1. Drill a 8.5 mm diameter hole in the installation location.
2. Use a threading tap to create a M10×1.5 thread in the hole.
3. Install the base of the cable gland in the hole and tighten with a 13 mm wrench.
4. Insert the seal of the cable gland in the base and place the nut of the cable gland over the probe head.

5. Insert the probe head in the cable gland up to the black plastic part of the probe head. Leave the black plastic part entirely outside the cable gland. Tighten the cable gland to finger tightness.
6. Tighten the nut of the cable gland with a 13 mm wrench until the probe head stops moving. Do not overtighten.

4.9.2 Overview of HMP9 Duct Installation Kit

Duct Installation Kit (Vaisala item ASM214055) is an optional accessory designed to support the probe head of a HMP9 Humidity and Temperature Probe in installations to ducts and chambers. The kit is lightweight and can be installed with minimal tools.

The kit does not include an attachment for the probe body of HMP9. To mount the probe body, use the probe holder supplied with HMP9, or attach it directly to a compatible Indigo transmitter.

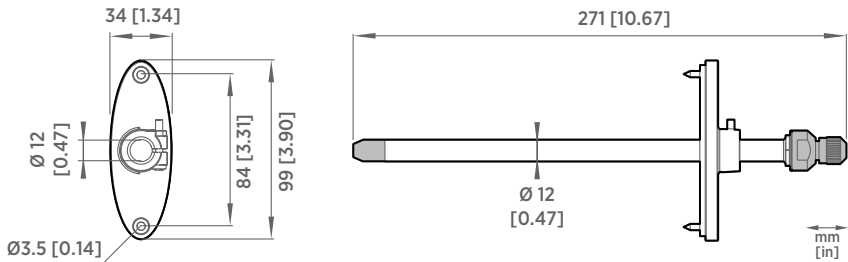


Figure 18 Duct Installation Kit ASM214055 dimensions


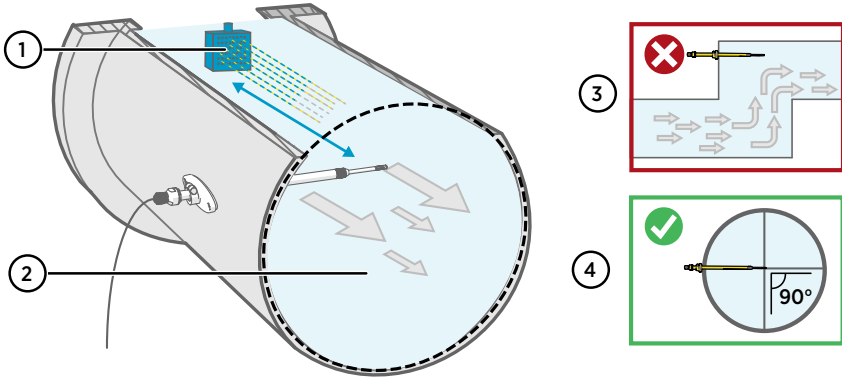


Figure 19 Duct installation overview




- 1 Make sure there is a minimum clearance of 5 m (16.5 ft) between the probe head and any possible humidifier. Avoid installing in a location where condensation can fall on the probe head inside the duct.
- 2 Maximum air flow speed: 50 m/s.
- 3 Avoid installing the probe in dead legs. Supersaturation can occur in areas where there is no air flow.
- 4 Install the probe head in a 90° angle to prevent condensation from travelling to the sensor along the mounting pipe. Position the sensor as close to the middle of the duct as possible.

4.9.3 Mounting HMP9 probe head with Duct Installation Kit


- ▶ 1. Loosen the sealing gland on the back of the pipe by turning it 1.5 full rotations. Do not detach the gland to avoid dislocating the sealing ring.

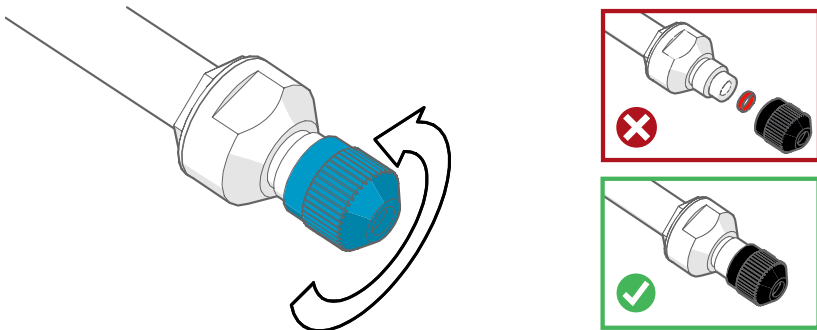

2. Push the probe head of HMP9 firmly through the sealing gland. Push the probe head further using its cable until it appears from the end of the tube. Adjust so that half of the metal probe head is visible, and tighten the sealing gland by hand so that it holds the probe cable in place.

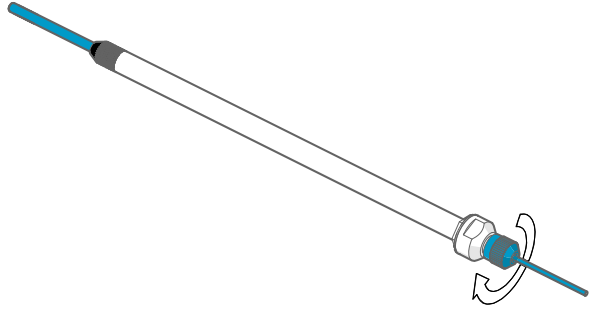

3. Insert the mounting flange on the pipe. Make sure the black sealing surface faces the probe head.
4. Make a \varnothing 14 mm (0.55 in) hole in the duct or chamber wall.
5. Push the probe head and pipe into the duct or chamber, and attach the flange using the 2 screws. If necessary, use a drill to make starter holes for the screws (max. \varnothing 2 mm (0.07 in)).
6. Adjust the mounting depth of the probe so that the probe is in the middle of the duct, and tighten the holding screw on the flange to lock the pipe in place.

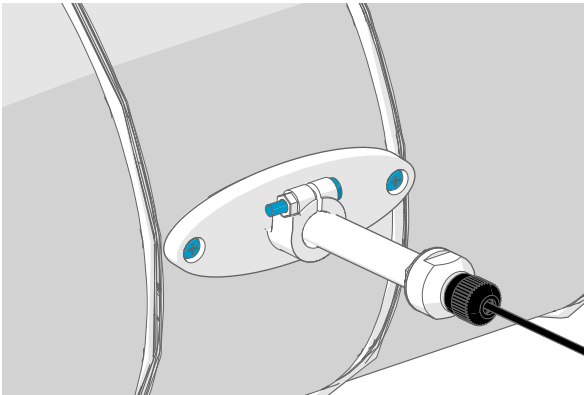

4.10 MMP8 probe

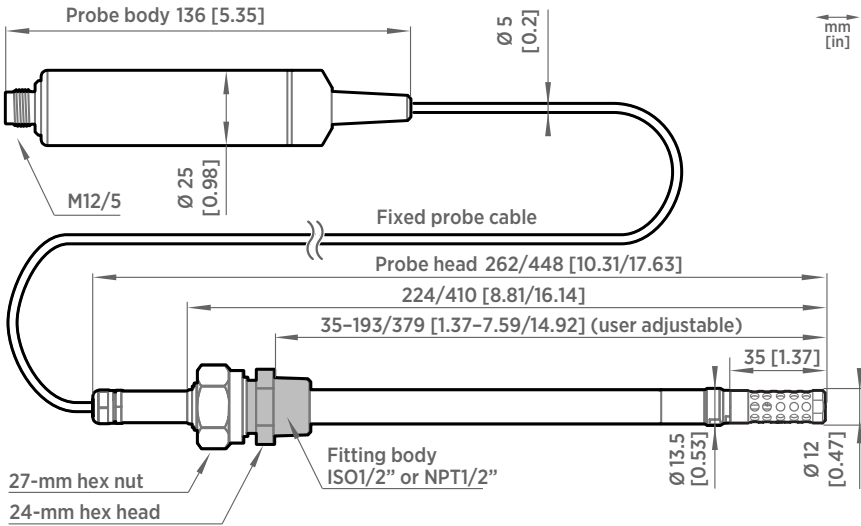


Figure 20 MMP8 dimensions

Vaisala HUMICAP® Moisture in Oil Probe MMP8 enables fast and reliable measurement of moisture in oil. It uses the proven Vaisala HUMICAP® sensor, which was developed for demanding dissolved moisture measurements in transformer and lubrication oils, hydraulic fluids, and other liquids.

MMP8 measures dissolved moisture in oil in terms of water activity (a_w), relative saturation (%RS), and temperature (T). Water activity or relative saturation indicate directly whether there is a risk of free water formation. This data is relevant in lubrication oil applications where detecting water ingress and preventing free water formation is crucial. The measurement is independent of oil type and age.

MMP8 can also output ppm, the average mass concentration of water in oil. Vaisala has this conversion readily available for specific oils, including mineral transformer oil. This allows continuous measurement of ppm concentration in power transformer condition monitoring.

- Temperature measurement range $-40 \dots +180 \text{ }^\circ\text{C}$ ($-40 \dots +356 \text{ }^\circ\text{F}$)

When installed with an optional ball valve kit, MMP8 is ideal for installation into processes where the probe needs to be installed or removed while the process is running. MMP8 is available in two different lengths, and the installation depth of the probe is adjustable. Pressure fitting options are ISO 1/2" and NPT 1/2". MMP8 is delivered with a manual pressing handle that allows the probe to be pushed against process pressure.

For more information on using the probe with the ball valve, see [Ball Valve Kit \(BALLVALVE-1\) Installation Guide \(M212837EN\)](#).

4.10.1 Moisture ppm calculation for transformer oils

MMP8 can also output ppm, the average mass concentration of water in oil. Vaisala has this conversion readily available for specific oils, including mineral transformer oil. This allows continuous measurement of ppm concentration in power transformer condition monitoring.

The table below lists the oil solubility coefficients of the oil types that can be used for the MMP8 probe.

Table 4 Oil solubility coefficients for Vaisala moisture in oil products

| Oil type | Oil 0 (A) | Oil 1 (B) |
|--|-----------|-----------|
| Mineral oils (for example, Shell Diala, Nynas Nytro) | -1662.70 | 7.3694 |
| Midel 7131 | -687.54 | 5.6236 |
| FR3 | -684 | 5.3318 |
| Dow Corning 561 | -1248.64 | 6.5427 |

After installing the MMP8 probe, configure the coefficients using the Insight PC software or the Indigo80 handheld indicator.


For determining the coefficients using your own apparatus, see [Determining Oil-specific Coefficients for Moisture in Oil Probes Technical Note \(M212935EN\)](#).

4.10.1.1 Configuring coefficients using Insight

After installation, you can configure coefficients for the MMP8 probe using the Insight PC software.



Configuring these settings requires using Insight in **Advanced Mode**.

- ▶ 1. Connect the probe to the Insight software.
2. Select  and open the **Configure device** menu.
3. Select **Calculation coefficients**.
4. In the **Oil A** and **Oil B** fields, enter the values of the required coefficients.
5. Select **Save**.

More information

- ▶ [Connecting to Insight software \(page 53\)](#)

4.10.1.2 Configuring coefficients using Indigo80

After installation, you can configure coefficients for the MMP8 probe using the Indigo80 handheld indicator.

- ▶ 1. Connect the probe(s) to the indicator.
2. Open the main menu by pressing (⊖).
3. Select **Devices**. If you have more than one device connected to the indicator, make a further selection between the devices.
4. Select **Settings** to access and change the features available for your probe.
5. Select **Calculation coefficients**.
6. Select **Oil A**, and use the arrow buttons to set the required value.
7. Select **Oil B**, and use the arrow buttons to set the required value.

More information

- ▶ [Connecting probes to Indigo80 \(page 64\)](#)

4.11 TMP1 probe

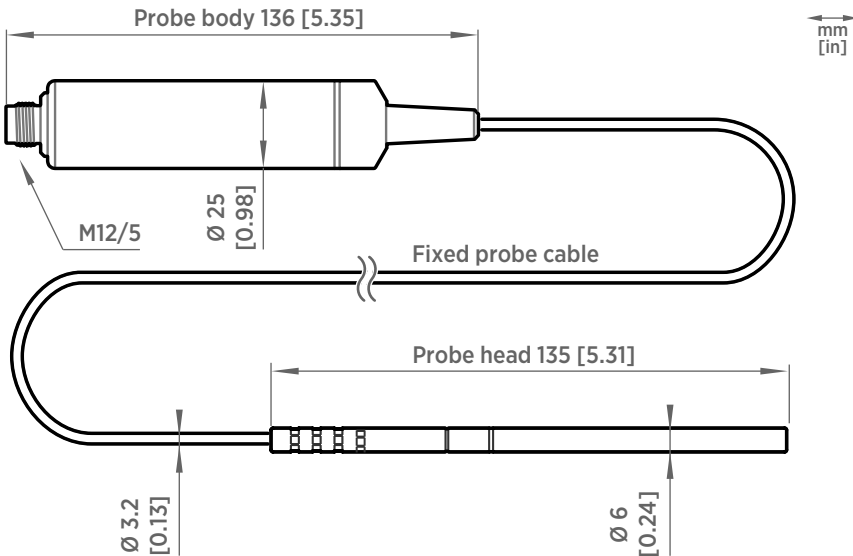


Figure 21 TMP1 probe dimensions

Vaisala Temperature Probe TMP1 is designed for demanding temperature measurements in industrial applications such as pharmaceutical industry and calibration laboratories, where accuracy and robustness are essential.

- Temperature measurement range $-70 \dots +180 \text{ }^{\circ}\text{C}$ ($-94 \dots +356 \text{ }^{\circ}\text{F}$)
- Operating temperature of probe body $-40 \dots +80 \text{ }^{\circ}\text{C}$ ($-40 \dots +176 \text{ }^{\circ}\text{F}$)

4.11.1 Duct installation kit for temperature probe

With an optional duct installation kit (Vaisala item 215003) to support the probe head, the probe can be installed to a chamber or duct.

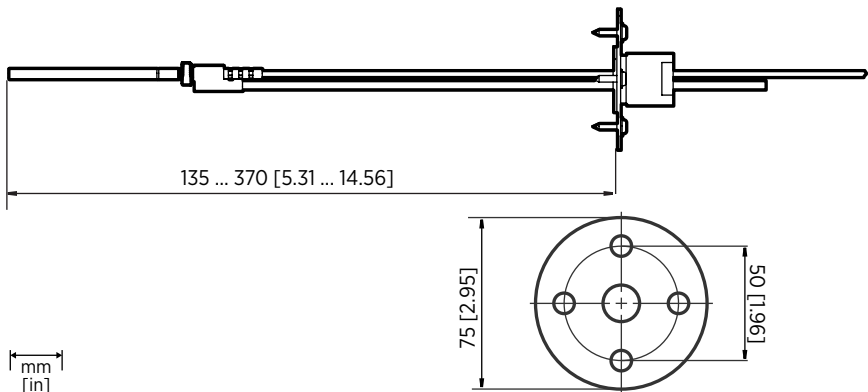


Figure 22 Optional duct kit 215003 dimensions

4.11.2 Pressure-tight Swagelok installation kit

Swagelok installation kit (Vaisala items SWG6ISO18 and SWG6NPT18) is an optional accessory which includes a pressure-tight Swagelok® connector with ISO1/8" or NPT1/8" thread.



CAUTION! Note that overtightening the connector may damage the probe head.

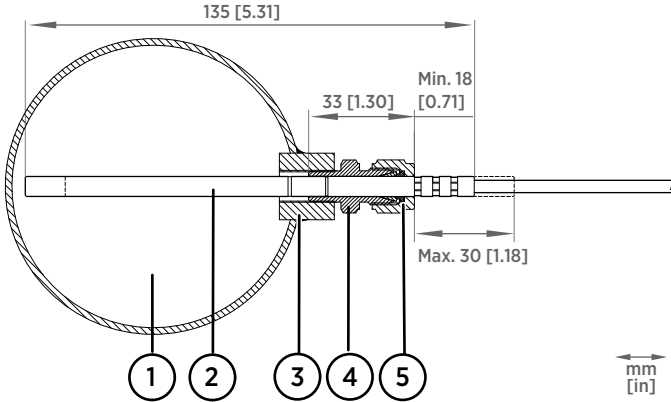


Figure 23 TMP1 installation to pipeline using a Swagelok installation kit

- 1 Max. process pressure 10 bar (145 psi), max temperature +180 °C (+356 °F)
- 2 Probe head
- 3 Duct connector
- 4 Swagelok connector
- 5 Ferrules

4.12 DTR502B solar radiation shield

DTR502B protects the sensors on the probe head from solar radiation and precipitation in outdoor installations. It provides excellent ventilation while blocking both direct and reflected solar radiation. The special plastic used in the plates has excellent thermal characteristics, the white outer surface reflects radiation, the black inside absorbs accumulated heat. The shield can be easily installed on either a vertical pole, horizontal beam, or a flat surface.

DTR502B is compatible with the probe heads of HMP3, HMP7 and HMP9 probes. HMP9 requires the use of a special sensor head support (item code 215130) due to the smaller diameter of its probe head.



DTR502B is designed to hold only the **probe head**. The probe body must be separately mounted and protected in outdoor installations. If possible, mount the probe indoors and bring only the probe head outside, into the DTR502B.

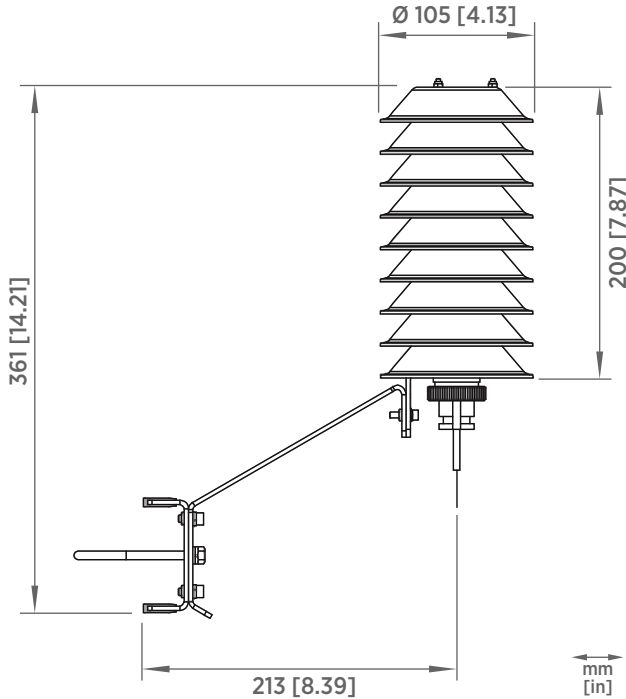


Figure 24 DTR502B dimensions

4.12.1 Mounting probe head inside DTR502B



- 3-mm and 5-mm Allen keys
- Crosshead screwdriver

DTR502B solar radiation shield is compatible with the probe heads of HMP3, HMP7, and HMP9 probes. The sensor head support that is included with the DTR502B is suitable for attaching HMP3 and HMP7 probe heads, but for HMP9 you need an alternate sensor head support (item code 215130).

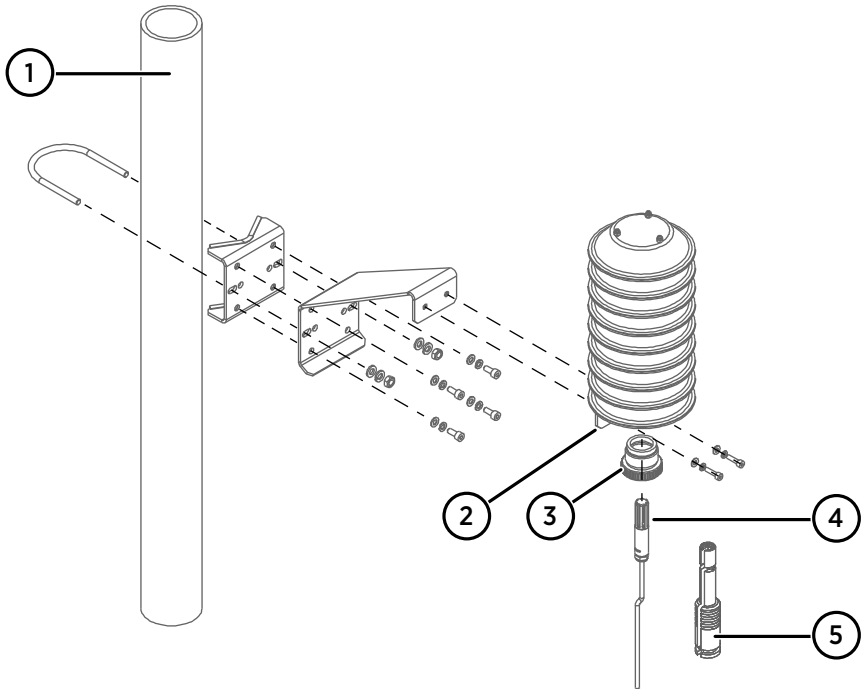


Figure 25 Mounting DTR502B on a pole mast

- 1 Pole mast with diameter 30–60 mm (1.2–2.3 in)
- 2 Support plate
- 3 Fastening ring
- 4 Probe head
- 5 Sensor head support

- ▶ 1. Mount the solar radiation shield in the measurement location using the provided mounting accessories, screws, and washers. You can mount the radiation shield to a pole mast as shown in [Figure 25 \(page 50\)](#), or to a horizontal beam directly from its support plate.

2. Attach the probe head to the sensor head support and secure it with a cable tie. The alternate sensor head support (item code 215130) needed with HMP9 is shown in [Figure 26 \(page 51\)](#).

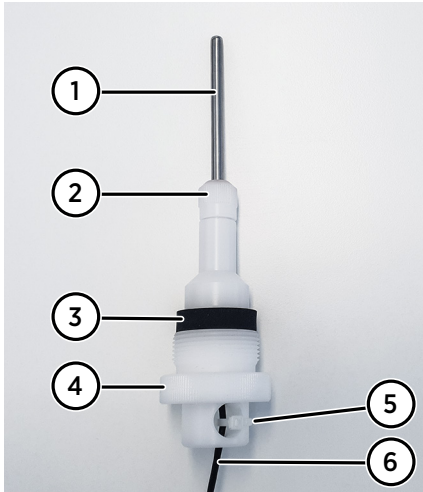


Figure 26 HMP9 probe head with sensor head support 215130

- 1 HMP9 probe head
- 2 Mounting nut
- 3 Sealing ring
- 4 Fastening ring
- 5 Cable tie
- 6 Cable between probe head and probe body

3. Insert the fastening ring and the sealing ring on the probe head.
4. Slide the probe head into the radiation shield and tighten the sealing ring.

4.13 Configuring environmental compensations

After installation, configure the pressure compensation setting, if relevant to your probe and its measurement environment.

For example, when you have installed the probe in a process with a pressure differing from normal atmospheric pressure, update the correct pressure into the pressure compensation setpoint parameter or register of the probe. This allows the probe to apply the appropriate pressure compensation into its measurement results.

You can configure the setting with the Insight software or the Indigo80 handheld indicator, or using the Modbus protocol.

More information

- [Environmental compensation \(page 23\)](#)
- [Environmental compensation \(page 23\)](#)
- [Configuring environment settings with Indigo80 handheld indicator \(page 67\)](#)

5. Configuration with Insight software

5.1 Vaisala Insight software

Vaisala Insight software is a configuration software for Indigo-compatible devices. With the Insight software, you can:

- See probe information and status
- See real-time measurement
- Record data up to 48 hours and export in CSV format
- Configure probe features such as measurement filtering, sensor purge, condensation prevention, and serial communication
- Calibrate and adjust the probe

Microsoft Windows® operating system and Indigo USB adapter (item code USB2) or Vaisala USB cable (item code 242659) required.

Download Vaisala Insight software at www.vaisala.com/insight.

5.2 Connecting to Insight software



- Computer with a Microsoft Windows® operating system (64-bit version) and Vaisala Insight PC software installed
- Indigo USB adapter (item code USB2) or USB connection cable (item code 242659)



CAUTION! When connecting several devices at the same time, note that your computer may not be able to supply enough power through its USB ports. Use an externally powered USB hub that can supply >2 W for each port.

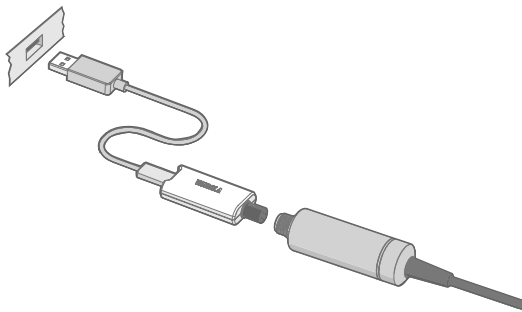



Figure 27 Connecting probe to Insight using Indigo USB adapter

- ▶ 1. Open the Insight software on your PC.
2. Verify the current operating mode of Insight from the **Settings** menu and change it if appropriate:
 - **Basic mode** is suitable for most use cases.
 - **Advanced mode** provides access to additional configuration options. Use **Advanced mode** only when instructed to do so by product documentation or Vaisala technical support.
3. Connect the USB adapter to a free USB port on the PC or USB hub.
4. Connect the probe to the USB adapter.
5. Wait for the Insight software to detect the probe.

5.3 Configuration options

The complete probe configuration is accessible via the Insight software. After connecting the probe, select  > **Configure device** to access the configuration options.

The available configuration options include all of the Modbus configuration registers and several additional options. If Insight has been set to **Advanced mode**, additional configuration options may be available. Use **Advanced mode** only when instructed to do so by product documentation or Vaisala technical support.

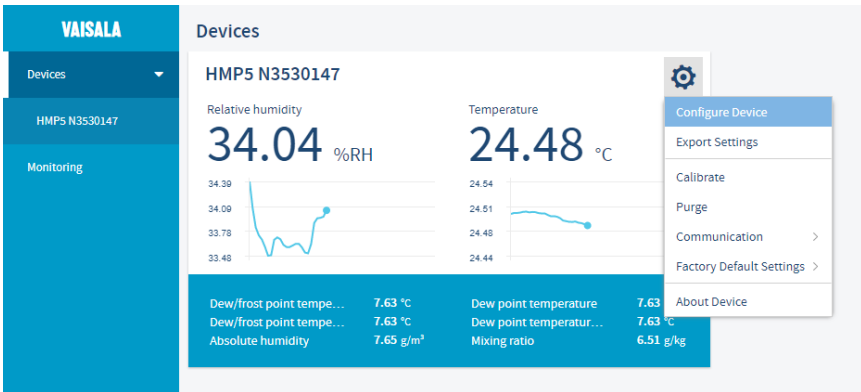


Figure 28 HMP5 in Insight software

5.4 Configuring condensation prevention with Insight

- ▶ 1. Connect the probe to the Insight software.

2. Select  > **Configure device**.
3. Set the **Condensation prevention on/off** switch to the desired setting.



The switch is not available if the probe does not support any condensation prevention heating features, or if the probe firmware version is older than 1.2.0. Probes with older firmware versions will show configuration switches for individual condensation prevention features as applicable.

More information

- [Connecting to Insight software \(page 53\)](#)
- [Condensation prevention functions \(page 22\)](#)

5.5 Diagnostics in Insight

Messages sent by the connected devices are shown automatically in Insight. Additional diagnostic data is available on the **Diagnostics** page. The data available depends on the probe model and Insight operating mode (basic or advanced). The data can be very useful when diagnosing issues together with Vaisala support, particularly the diagnostic files.

Diagnostic files

If Insight is in **Advanced mode**, you can retrieve the following diagnostic files from the connected probe:

- **SSR/T, histogram**: Table of humidity and temperature conditions measured by the probe
- **Error log**: Cumulative total of the error and status events tracked by the probe

Both files contain data from since the probe was manufactured, or since the files were last cleared. Clearing the files is not recommended unless instructed by Vaisala support. The buttons to clear the files are located at the bottom of the **Diagnostics** page.

The files are in comma separated value (CSV) format. They can be opened for viewing in spreadsheet programs such as Microsoft Excel or in text editors.

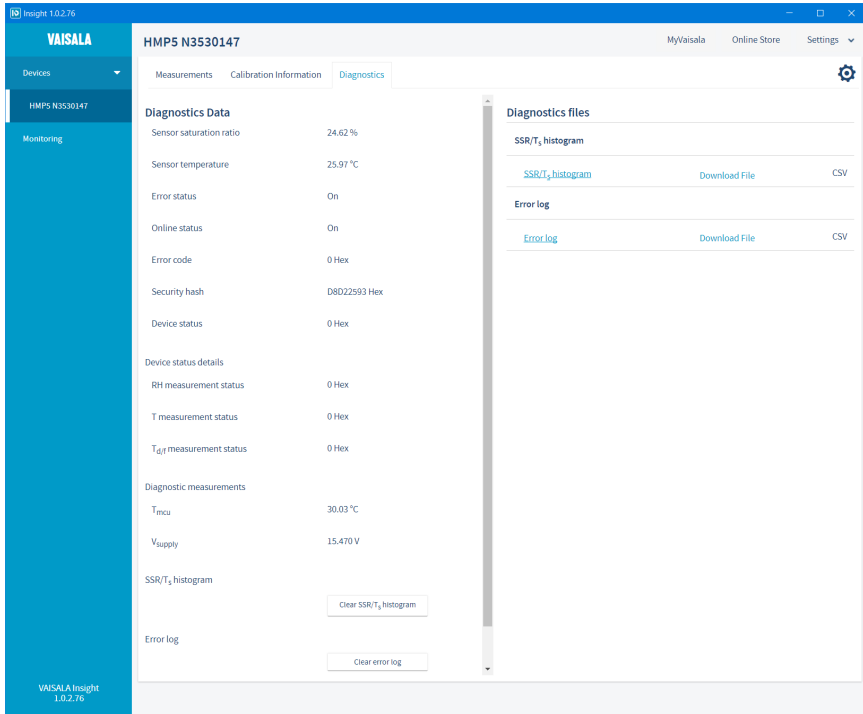


Figure 29 HMP5 diagnostics in Insight (advanced mode)

6. Using probe with Indigo transmitters

Indigo transmitters are host devices that extend the feature set of connected probes with a range of additional options for outputs, configuration access, measurement viewing, and status monitoring.

Available features vary depending on the transmitter model. Models without display use a LED indicator for notifications.

For more information on the features of the different Indigo transmitter models, see www.vaisala.com/indigo.

For instructions on installing and configuring Indigo transmitters, see the applicable Indigo transmitter user documentation available at the Vaisala documentation portal docs.vaisala.com.

6.1 Connecting probe to Indigo200 series transmitters

Indigo200 series transmitters have a probe connector where compatible probes can be attached directly. A cable may also be used to connect the probe. Cables are available to order at store.vaisala.com.



CAUTION! The IP classification of probes is valid only when the probes are connected to the probe connection cable, or to the cable connector inside the locking wheel of the transmitter.

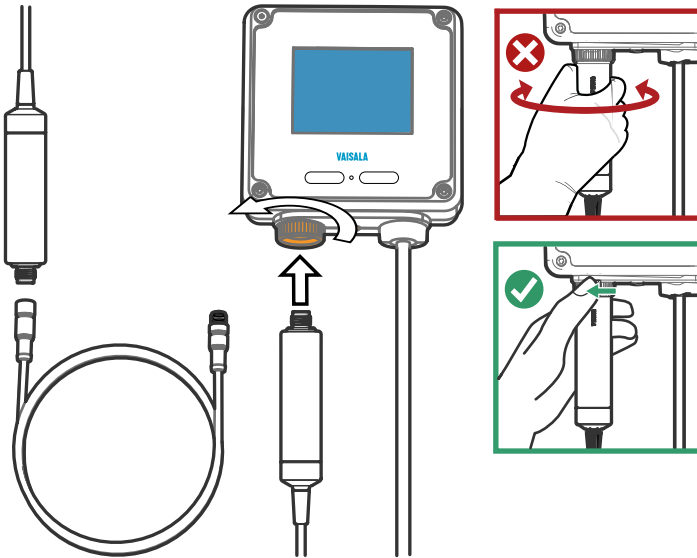


Figure 30 Connecting probe to Indigo200 series transmitter

- ▶ 1. Insert the probe or the cable into the transmitter's connector. Using a cable is recommended for strain relief.
2. Turn the locking wheel of the transmitter to lock the probe or cable in place. **Do not turn the probe or the cable itself**, as that will damage the connectors.
3. If you are using a cable, connect the probe to the cable.
4. When the transmitter recognizes the connected probe, it shows a notification message on the display.

6.2 Connecting probe to Indigo300 transmitter

Indigo300 transmitters have a probe connector where compatible probes can be attached directly. A cable may also be used to connect the probe. Cables are available to order at store.vaisala.com.



CAUTION! The IP classification of probes is valid only when the probes are connected to the probe connection cable, or to the cable connector inside the locking wheel of the transmitter.

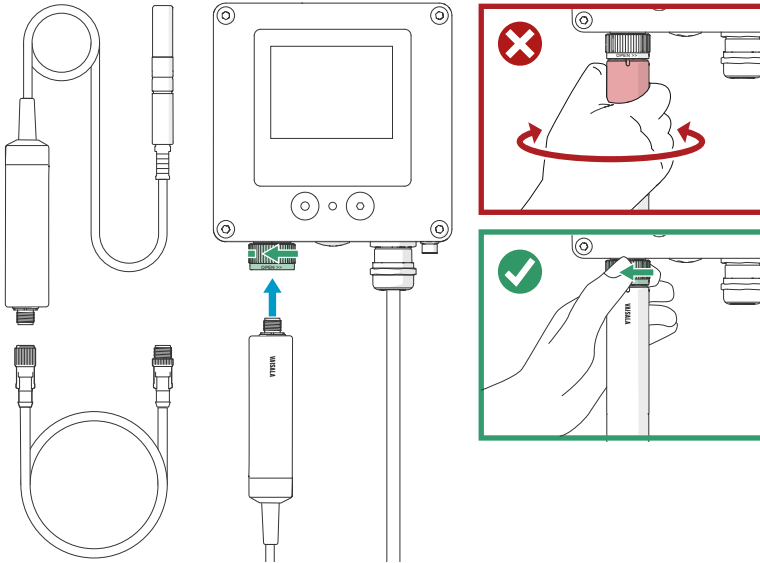


Figure 31 Connecting probe to Indigo300 transmitter

- ▶ 1. Insert the probe or the cable into the transmitter's connector.
2. Turn the locking wheel of the transmitter to lock the probe or cable in place. **Do not turn the probe or the cable itself**, as that will damage the connectors.
3. If you are using a cable, connect the probe to the cable.
4. When the transmitter recognizes the connected probe, it shows a notification message on the display.

6.3 Connecting probes to Indigo500 series transmitters



CAUTION! The IP classification of probes is valid only when the probes are connected to the probe connection cable.



If your transmitter was delivered with preconfigured analog outputs, make sure that you connect the measurement devices accordingly.

Probes are connected to Indigo500 series transmitters using a cable. Connections are made to the screw terminals inside the housing. The Indigo520 model allows 2 probes to be connected. After connecting a probe, use the touchscreen interface or the web user interface to configure the transmitter.

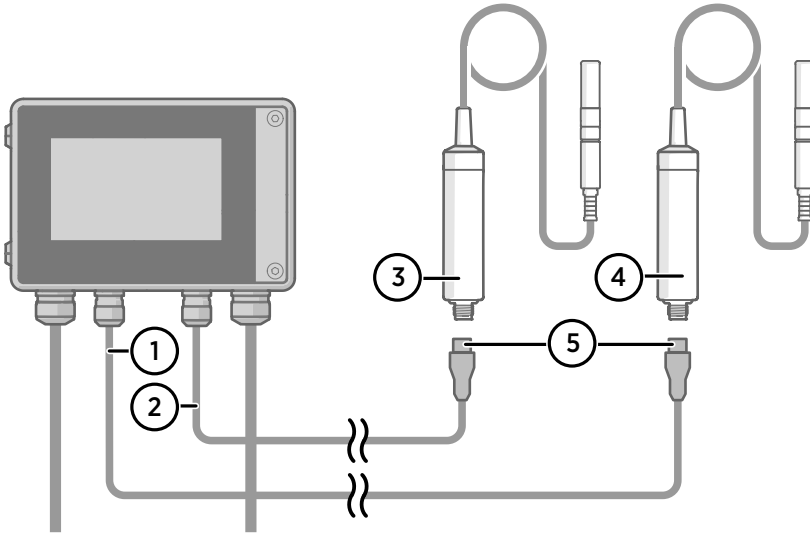


Figure 32 Connecting probes to Indigo500 transmitter

- 1 Probe connection cable for probe 1
- 2 Probe connection cable for probe 2 (dual-device support in Indigo520)
- 3 Probe to be connected as probe 2 (GMP252 example)
- 4 Probe to be connected as probe 1 (HMP7 example)
- 5 Probe cable connector (M12 5-pin A-coded female)

6.4 Default analog output configuration with Indigo transmitters

When you connect the probe to an Indigo200 or Indigo300 transmitter for the first time, the following analog output values per output parameter are active by default, unless you have ordered the transmitter with preconfigured analog outputs.

Table 5 Default analog output configuration per output parameter

| Output parameter | Output unit | AOUT min | AOUT max |
|-------------------|------------------|----------|----------|
| Absolute humidity | g/m ³ | 0 | 600 |

| Output parameter | Output unit | AOUT min | AOUT max |
|--------------------------------------|------------------|----------|-----------|
| Absolute humidity at NTP | g/m ³ | 0 | 600 |
| Dew/frost point temperature | °C | -80 | 100 |
| Dew/frost point temperature at 1 atm | °C | -80 | 100 |
| Dew point temperature | °C | -80 | 100 |
| Dew point temperature at 1 atm | °C | -80 | 100 |
| Dew point temperature difference | °C | -10 | 50 |
| Enthalpy | kJ/kg | -40 | 1500 |
| Mixing ratio | g/kg | 0 | 500 |
| Relative humidity | %RH | 0 | 100 |
| Relative humidity (dew/frost) | %RH | 0 | 100 |
| Relative saturation | %RS | 0 | 100 |
| Temperature | °C | -40 | 60 |
| Water activity | - | 0 | 1 |
| Water concentration | ppm _v | 0 | 1 000 000 |
| Water concentration in oil | ppm _w | 0 | 1 000 000 |
| Water concentration (wet basis) | vol-% | 0 | 100 |
| Water mass fraction | ppm _w | 0 | 1 000 000 |
| Wet-bulb temperature | °C | 0 | 100 |
| Water vapor pressure | hPa | 0 | 1000 |
| Water vapor saturation pressure | hPa | 0 | 1000 |

7. Using probe with Indigo80 handheld indicator

7.1 Indigo80 handheld indicator

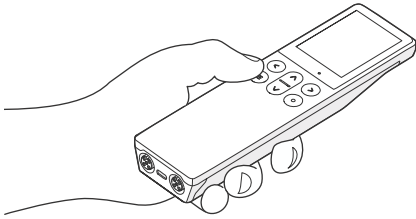


Figure 33 Indigo80 handheld indicator


Vaisala Indigo80 Handheld Indicator is a portable diagnostics tool that accommodates up to two Vaisala Indigo-compatible probes or transmitters for measuring a wide range of parameters.

With the indicator, you can:

- See real-time measurements and device and status information
- Log measurement data
- Calibrate and adjust the probe
- Configure probe features and settings such as condensation prevention, compensation setpoints, sensor purge, filtering factor, and serial communication. The available features and settings depend on the probe model and firmware version.
- Enable temperature compensation from another probe. For example, you can enable TMP1 to function as the temperature source for HMP7.



Accessing certain configuration options for your probe requires using the free Insight PC software, downloadable at www.vaisala.com/insight.

The help tours in the indicator's user interface guide you through the key features of the indicator. You can access the tours in the **Help** menu by pressing the  button.

For more information on using the indicator, for example, editing the measurement views and performing data logging, see [Indigo80 User Guide \(M212722EN\)](#).

More information

- [Configuring probe features with Indigo80 handheld indicator \(page 66\)](#)
- [Configuring environment settings with Indigo80 handheld indicator \(page 67\)](#)
- [Calibration and adjustment with Indigo80 handheld indicator \(page 76\)](#)

7.1.1 Probe compatibility

The Indigo80 handheld indicator is tested for compatibility with probes that have firmware version 1.2.5 or newer.

Probes with older firmware versions may have limited compatibility with the indicator.

For the most up-to-date version compatibility information, see [Indigo80-compatible Firmware Technical Note \(M212901EN\)](#).

7.1.2 Indigo80 keypad

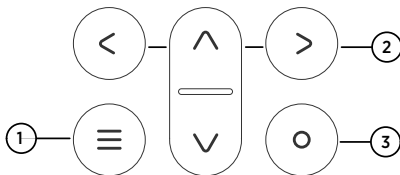


Figure 34 Indigo80 keypad

- 1 Power on/off and main menu button
- 2 Arrow buttons for navigating menus and scrolling views
- 3 Select button for selecting items in the user interface

7.1.3 Indigo80 main menu

Pressing the  button while navigating the Indigo80 menus and views opens the main menu.

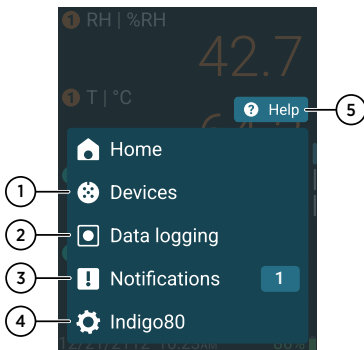


Figure 35 Indigo80 main menu

- 1 **Devices** menu contains, for example, options related to sensor purge, calibration, and environment settings (depending on the connected device).
- 2 **Data logging** menu for setting logging interval and duration, and browsing data files.
- 3 **Notifications** menu displays notifications related to Indigo80 and the connected devices.
- 4 **Indigo80** menu for changing the settings of Indigo80 (for example, date, time, and language) and viewing device information.
- 5 **Help** menu contains tours showing the key features of Indigo80, as well as instructions for sending devices to Vaisala for calibration and maintenance.

7.2 Connecting probes to Indigo80



- Probe connection cable

Up to two Vaisala Indigo-compatible probes or transmitters can be connected to the ports located on the bottom of Indigo80. You can connect and disconnect devices both when the indicator is powered on and when it is off.

Vaisala recommends using cables provided by Vaisala when connecting devices to the indicator. Cables and other accessories are available to order at store.vaisala.com.

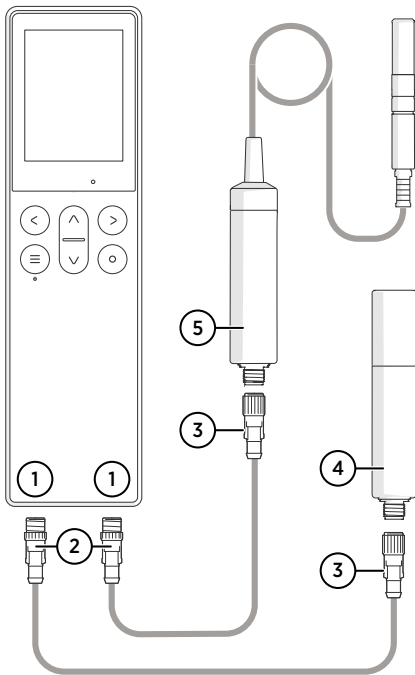




Figure 36 Connecting probes to Indigo80

- 1 M12-5F ports on the bottom of Indigo80 for connecting compatible Vaisala devices. Ports are labeled ① and ②.
- 2 M12-5M A-coded cable connector
- 3 M12-5F A-coded cable connector
- 4 Probe displayed as ① by Indigo80 (GMP252 shown)
- 5 Probe displayed as ② by Indigo80 (HMP7 shown)


- ▶ 1. If the indicator is powered and no devices are connected to it, the text **Please connect a probe** will be shown on the display.

2. Insert the probe connection cable in one of the ports on the bottom of the indicator.

- **Note the orientation of the cable connector when inserting it**
- **Hold the connector in place while turning its locking ring clockwise – never twist the connector body!**

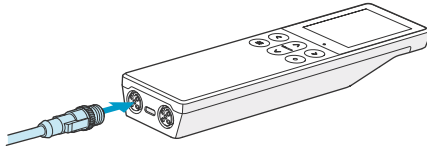

3. Connect the probe to the M12-5F end of the probe connection cable.



When the indicator recognizes the connected probe, it shows a notification on the display (for example, **GMP252 connected**). A probe connected to the leftmost port in the indicator is labeled **1** on the indicator's display, while the probe in the rightmost port is labeled **2**.

4. To change probes, simply detach the cable from the probe and connect a new probe.



For optimal measurement accuracy, the indicator guides you to check the connected probe's environment settings next.

More information

- [Configuring environment settings with Indigo80 handheld indicator \(page 67\)](#)

7.3 Configuring probe features with Indigo80 handheld indicator



- Probe connection cable

You can use the Indigo80 handheld indicator to configure probe features such as compensation setpoints, filtering factor, and serial communication. The available features depend on the probe model and firmware version.



Accessing certain configuration options for your probe requires using the free Insight PC software, downloadable at www.vaisala.com/insight.

- ▶ 1. Connect the probe(s) to the indicator.
2. Open the main menu by pressing
3. Select **Devices**. If you have more than one device connected to the indicator, make a further selection between the devices.
4. Select **Settings** to access and change the features available for your probe.
5. Exit the menu by pressing or return to the main menu by pressing .

More information

- [Sensor purge \(page 21\)](#)
- [Condensation prevention functions \(page 22\)](#)
- [Environmental compensation \(page 23\)](#)
- [Filtering factor \(page 24\)](#)

7.3.1 Example of configuring filtering factor with Indigo80 handheld indicator






- Probe connection cable

The filtering factor allows averaging the output if the measuring environment produces occasional exceptionally high or low readings.

This example shows how to configure the filtering factor as **0.9** using the Indigo80 handheld indicator.

This means that the new measurement output is a combination of the latest measurement (90 %) and the previous measurement (10 %).

- ▶ 1. Connect the probe(s) to the indicator.
2. Open the main menu by pressing .
3. Select **Devices**. If you have more than one device connected to the indicator, make a further selection between the devices.
4. Select **Settings > Filtering**.
5. Select **Filtering factor**.
 - a. Use the arrow buttons to set the value as **0.9**.
 - b. Select **Set**.
6. Select **Extended filtering on/off > On** to enable measurement filtering using the filtering factor defined in the previous step.
7. Exit the menu by pressing  or return to the main menu by pressing .

More information

- [Filtering factor \(page 24\)](#)

7.4 Configuring environment settings with Indigo80 handheld indicator



- Probe connection cable


For optimal measurement accuracy, you can use the Indigo80 handheld indicator to give additional information about the connected probe's measurement environment.

For example, you can:

- Configure the pressure compensation setting for your probe
- Enable temperature compensation from another Indigo-compatible probe that has a temperature output. For example, you can enable TMP1 to function as the temperature source for HMP7.



The environment settings available through Indigo80 correspond to the environmental compensation settings of the probe. Therefore, **Environment settings** and **Settings > Compensation setpoints** are interconnected: the configuration set in either menu is applied to both.

- ▶ 1. Connect the probe(s) to the indicator.
2. Open the main menu by pressing .

3. Select **Devices**. If you have more than one device connected to the indicator, make a further selection between the devices.
4. Select **Environment settings** to access the settings for your probe.

The available environment settings depend on the probe and probe firmware version.

Pressure

Value for pressure compensation. The entered value is persistent and remains unchanged at device restart.

Temperature



This setting allows the probe to use a temperature reading from another device instead of its own temperature reading. An external temperature source is needed when condensation prevention functions of the probe are active, as they will also heat the temperature sensor of the device. Indigo80 can link a temperature measurement from another probe to this setting and update it in real time.



Some probe firmware versions may allow a value to be entered manually. This is not recommended as the value must correspond to the temperature of the measurement environment as accurately as possible.



A manually entered value is cleared at device reset. A value read from another probe is persistent: when you disconnect and then reconnect the same probes to the same ports in Indigo80, Indigo80 will continue reading the temperature value from the previously selected probe. The same applies also when you restart Indigo80 with the same probes connected.

5. Select a setting from the list, for example, **Pressure**.
 - a. Select the unit, if prompted.
 - b. Use the arrow buttons to set the desired value, and then select **OK** or **Set**.

You can also select to read the value from another probe connected to the indicator, provided that the probe can output the required compensation parameter. Press  to highlight the **Read value from** field, and then press  to select the other probe as the source of the value.



For **Temperature**, always set the temperature value to be read from another probe. Do not set the temperature value manually. Make sure that both probes are in the same environment to get the most accurate measurement values.

- Exit the menu by pressing  or return to the main menu by pressing .

More information

- [Pressure compensation \(page 23\)](#)
- [Temperature compensation \(page 23\)](#)
- [Example of enabling temperature compensation with Indigo80 handheld indicator \(HMP7 and TMP1\) \(page 69\)](#)

7.4.1 Example of enabling temperature compensation with Indigo80 handheld indicator (HMP7 and TMP1)




- Probe connection cable (2 pcs)

The temperature-dependent output parameters of the HMP7 humidity and temperature probe are unavailable when the probe heating function of HMP7 is active. Therefore the temperature measurement data needs to be provided from an external source, which can be, for example, any Indigo-compatible probe with a temperature output. With HMP7 and TMP1 connected to the Indigo80 handheld indicator, you can enable TMP1 to function as the temperature source for HMP7.




Make sure that both probes are in the same environment to get the most accurate measurement values.

- ▶ 1. Connect the probe(s) to Indigo80 in any order.
In this example, TMP1 is connected to port 1 of the indicator, and HMP7 to port 2.
2. Open the main menu by pressing .
3. Select **Devices > HMP7**.
4. Select **Environment settings > Temperature**.

5. Select **Read from device > TMP1**.

The temperature value read from TMP1 is now shown in the **Environment settings** of HMP7.



To stop reading the temperature value from TMP1, select **HMP7 > Environment settings > Temperature > Stop reading**.

6. Exit the menu by pressing ⏪ or return to the main menu by pressing ⏩.



When you disconnect and then reconnect the same probes to the same ports in Indigo80, Indigo80 will continue reading the temperature value from the previously selected probe. The same applies also when you restart Indigo80 with the same probes connected.

More information

- [Temperature compensation \(page 23\)](#)

8. Calibration and adjustment

8.1 Calibration and adjustment overview



Calibration means comparing the measurement output of the device to a known reference, such as a known environment in a calibration chamber or the output of a reference instrument. Correcting the reading of the device so that it measures accurately is referred to as **adjustment**.

The probe is fully calibrated and adjusted as shipped from the factory, and a calibration reminder with a 12-month interval is activated in the probe. To maintain the accuracy of the measurement, calibrate and adjust the probe as indicated by the calibration reminder, or as needed. Typical calibration interval is one year, but depending on the application it may be necessary to check the accuracy more frequently.

Vaisala recommends sending the probe regularly to Vaisala for factory calibration. The probe is calibrated and adjusted at multiple points along its measurement range. Factory calibration always includes a traceable calibration certificate and adjustment, if needed.

Factory calibration leads to highest accuracy and lowest uncertainty. After factory calibration the instrument performs as new. For up-to-date information about calibration points and offering, visit store.vaisala.com.



WARNING! When returning a product for calibration or repair, make sure it has not been exposed to dangerous contamination, and is safe to handle without special precautions.

It is also possible to calibrate and adjust the probe on the field using the Insight PC software, the Indigo80 handheld indicator, or via an Indigo transmitter that is connected to Insight or Indigo80. You can also modify the probe's calibration interval and reminder using the above-mentioned tools.



If you think the device is not measuring correctly, calibration and adjustment is not the first thing to do. Check the following first:

- Make sure nothing is interfering with the measurement: heat sources, temperature differences, or condensation.
- Check that there is no moisture on the probe. If the sensor has become wet, wait for it to dry.
- Always wait for the measurement to stabilize.

8.2 Adjustment points and requirements

You can adjust the humidity measurement in 1 ... 5 points and temperature measurement in 1...2 points, depending on the device that you use for the adjustment. Note the following:

- Humidity adjustment in more than 2 points is only available when you use the Insight software in **Advanced Mode**.
- If you are adjusting in more than one humidity point, make sure the first two points are at least 10 %RH apart.
- The probe will reject adjustments that are too large, that is, greater than 10 %RH for humidity and 0.5 °C for temperature. If the probe appears to need such a large correction, perform a sensor purge and repeat the adjustment procedure. Make sure that the measurement has stabilized and the reference environment is reliable. If the required adjustment is still too large, the probe needs to be serviced by Vaisala.



When adjustment of humidity measurement is necessary, Vaisala recommends adjusting in two points, 11 %RH and 75 %RH. These humidities can be produced using Vaisala HMK15 Humidity Calibrator. Adjustment of temperature measurement is typically not necessary.

8.3 HMK15 Humidity Calibrator with HMP Series probes

Vaisala HMK15 Humidity Calibrator is a suitable humidity reference for HMP Series probes. When preparing the salt solutions and using the calibrator, follow the general instructions in the *HMK15 User Guide (M210185EN)* to avoid common sources of calibration error.

HMK15 with HMP3, HMP4, HMP5, HMP7, and HMP8 probes

Before inserting the probe head in the salt jar, remove the filter and inspect the sensor element. If the leg pins of the sensor are longer than 7 mm (0.28 in), attach the 211302SP calibration adapter. This prevents the sensor from being submerged in the salt solution. Composite sensors typically have long leg pins.

211302SP is the longer of the two adapters included with HMK15. With this adapter attached, use the 13.5 mm hole on the salt jar cover.



Figure 37 HMP5 calibration with HMK15 using 211302SP adapter

12 mm (0.47 in) diameter probes where the leg pins are shorter than 7 mm can be inserted in the salt jar without an adapter. Note that you can still use the 218377SP calibration adapter to fit a 12 mm probe in the 13.5 mm hole. This allows you to have multiple probes inserted in a salt jar at one time.



CAUTION! Sensors on the probe head are vulnerable to damage when the filter is removed. Handle the probe carefully and avoid touching the sensors.

HMK15 with HMP1 and HMP9

HMP9 calibration adapter for HMK15 (item code ASM213801) is required to fit the HMP9 probe head to the 12 mm hole on the HMK15 salt jar.



Figure 38 Using HMP9 calibration adapter with HMK15

The same adapter does mechanically fit the HMP1 as well. However, use of HMK15 with HMP1 is not recommended due to additional temperature error caused by heat conduction from the electronics of the probe body. HMP1 should be calibrated so that the entire device is in the calibration environment, not just the probe head. Vaisala's calibration service is a good option for maintaining the accuracy of HMP1.



You can use HMK15 with HMP1 and achieve an accurate calibration if the probe is unpowered during stabilization. This is typically only practical for 1-point calibration.



8.4 Adjusting measurement with Insight software



- Computer with a Microsoft Windows® operating system (64-bit version) and Vaisala Insight PC software installed
- Indigo USB adapter (item code USB2) or USB connection cable (item code 242659)
- Reference environment(s) for producing the desired humidity and/or temperature

This procedure can be used to adjust the probe's humidity or temperature measurement. If you want to adjust both, repeat the procedure.

Because stabilization of temperature and humidity takes time, you should expect the adjustment procedure to take at least 30 minutes for each adjustment point.

1. Connect the probe to the Insight software.
2. If you intend to adjust humidity measurement, first select  > **Sensor purge** to perform sensor purge to condition the sensor. Wait a few minutes for purge to complete.
3. Select  > **Calibrate > Yes** to switch the probe to calibration mode.

In calibration mode, the device will not use functions that may interfere with calibration and adjustment.

4. Select the type of adjustment to perform: **RH adjustment** or **T adjustment**.
5. Define the needed adjustment for the first measurement point:
 - a. Insert the probe head in the reference environment for the first calibration point.
 - b. Wait for the measurement to stabilize fully. This may take more than 30 minutes. Monitor the readings to see when both the RH and temperature measurements have stabilized.
 - c. Click the **Reference value, point 1** text box and enter the reference value of the calibration point. Press **ENTER** or click outside the text box when done.
 - d. The probe automatically enters the measured values for the calibration point.
6. If you want to adjust in more than one point, repeat the previous step for all desired calibration points.



You can adjust humidity measurement in up to five points when Insight is set to **Advanced mode**.

7. Check the difference between each reference and measured value. Very large differences may be due to insufficient stabilization time or unsuitable calibration setup.
 - To save the adjustment into the device, select **Activate adjustment**.
 - To exit without taking the adjustment in use, select **Close**.

8. Check the message that appears at the top of the screen. If the message indicates that the adjustment is activated successfully, your adjustment is stored in the probe.
9. Select the **Calibration information** tab and update the **Calibration date** and **Calibration text**.
10. Select **Close** to exit the calibration mode.

More information

- [Connecting to Insight software \(page 53\)](#)
- [Adjustment points and requirements \(page 71\)](#)

8.5 Adjusting measurement with Indigo transmitter





- Reference environment(s) for producing the desired humidity and/or temperature
- Computer with a Microsoft Windows® operating system (64-bit version), Vaisala Insight PC software, and Vaisala USB Device driver installed
- For Indigo200 series transmitters: USB cable with a USB-C (type C to A or type C to C) connector (available as an accessory, a generic cable can also be used)
- For Indigo300 transmitter: M12 - M8 service cable (Vaisala item code 262195)

This procedure can be used to adjust the humidity or temperature measurement of a probe connected to an Indigo200 or Indigo300 transmitter, when the transmitter is connected to the Insight PC software.

Because stabilization of temperature and humidity takes time, you should expect the adjustment procedure to take at least 30 minutes for each adjustment point.

Indigo200 transmitters manufactured before 2022 have a wireless configuration interface for adjusting measurements. For more information, see version G of [HMP Series with MMP8 and TMP1 User Guide \(M212022EN\)](#).

- ▶ 1. Connect the transmitter to the Insight software.
The transmitter has a port on the lower right corner of the front panel.
2. If you intend to adjust humidity measurement, first select  > **Sensor purge** to perform sensor purge to condition the sensor. Wait a few minutes for purge to complete.
3. Select  > **Calibrate** > **Yes** to switch the probe to calibration mode.
In calibration mode, the device will not use functions that may interfere with calibration and adjustment.
4. Select the type of adjustment to perform: **RH adjustment** or **T adjustment**.

5. Define the needed adjustment for the first measurement point:
 - a. Insert the probe head in the reference environment for the first calibration point.
 - b. Wait for the measurement to stabilize fully. This may take more than 30 minutes. Monitor the readings to see when both the RH and temperature measurements have stabilized.
 - c. Click the **Reference value, point 1** text box and enter the reference value of the calibration point. Press **ENTER** or click outside the text box when done.
 - d. The probe automatically enters the measured values for the calibration point.
6. If you want to adjust in more than one point, repeat the previous step for all desired calibration points.



You can adjust humidity measurement in up to five points when Insight is set to **Advanced mode**.

7. Check the difference between each reference and measured value. Very large differences may be due to insufficient stabilization time or unsuitable calibration setup.
 - To save the adjustment into the device, select **Activate adjustment**.
 - To exit without taking the adjustment in use, select **Close**.
8. Check the message that appears at the top of the screen. If the message indicates that the adjustment is activated successfully, your adjustment is stored in the probe.
9. Select the **Calibration information** tab and update the **Calibration date** and **Calibration text**.
10. Select **Close** to exit the calibration mode.

More information

- [Adjustment points and requirements \(page 71\)](#)

8.6 Calibration and adjustment with Indigo80 handheld indicator

The Indigo80 handheld indicator provides two ways to calibrate and adjust measurements for probes: **Guided calibration** and **Manual adjustment**.

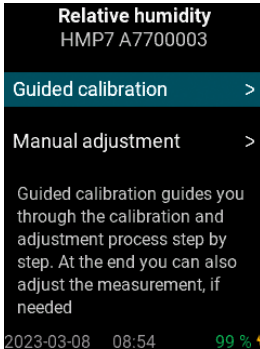


Figure 39 Indigo80 calibration methods for probes

- Choose **Guided calibration** when you want the indicator to guide you through the calibration process step by step. At the end you can also adjust the measurement, if needed.
- Choose **Manual adjustment** when you want to freely set the reference and measured values to adjust the measurement.

Calibrating a measurement with the indicator, including purge and adjustment, typically takes 1 to 2 hours depending on the number of calibration points.

8.6.1 Performing guided calibration with Indigo80 handheld indicator



- Probe connection cable
- Reference environment(s) for producing the desired reference values

In guided calibration, the indicator guides you through the calibration process step by step. At the end, you can also adjust the measurement, if needed.

You can choose to do either 1-point or 2-point calibration, and choose to use the reference environment or instrument of your choice, for example, another probe connected to your indicator.

For relative humidity, you can choose to use Vaisala HMK15 Humidity Calibrator. For more information on HMK15, see [HMK15 User Guide \(M210185EN\)](#).

- ▶ 1. Connect the probe(s) to the indicator.
2. If your probe supports the sensor purge feature, wait for the start-up purge to finish.
3. Open the main menu by pressing \ominus .
4. Select **Devices**. If you have more than one device connected to the indicator, make a further selection between the devices.
5. Select **Calibrate / Adjust**.

6. Select the type of calibration or adjustment to perform, for example, **RH adjustment**.
7. Select **Guided calibration**.
8. In **Calibration points**, select the number of the calibration points: **1 point** or **2 points**.
9. In **Reference**, select the desired reference environment(s) or reference instrument(s).

Selection **Other reference** allows you to use any reference environment(s) of your choice. For 2-point calibration of relative humidity, you can select two salts from the list, one for each calibration point.

When you have selected the reference environments for 2-point calibration, press ⏪ to get back to the previous view.

10. Select **Start calibration**.

The indicator guides you through the calibration process from this point onwards. Press ⏩ to proceed from one view to another.

More information

- [Connecting probes to Indigo80 \(page 64\)](#)
- [Adjustment points and requirements \(page 71\)](#)
- [HMK15 Humidity Calibrator with HMP Series probes \(page 72\)](#)

8.6.2 Performing manual adjustment with Indigo80 handheld indicator



- Probe connection cable
- Reference environment(s) for producing the desired reference values

This procedure tells you how to use the indicator to adjust the probe's measurement in 1–2 points. You can monitor the measurement graph shown by the indicator to determine the reference value and measured value for your calibration points. Alternatively, you can just enter predetermined values that you already have available.

Before you start, familiarize yourself with information on adjustment points and requirements for your probe.


- ▶ 1. Connect the probe(s) to the indicator.
2. Open the main menu by pressing ⏪.
3. Select **Devices**. If you have more than one device connected to the indicator, make a further selection between the devices.
4. If your probe supports the sensor purge feature, wait for the start-up purge to finish or start the purge manually by selecting **Devices > <your device> > Sensor purge**.

After the purge has been completed, continue to the next step.


5. Select **Calibrate / Adjust**.
6. Select the type of calibration or adjustment to perform, for example, **RH adjustment**.





7. Select **Manual adjustment**.
8. Place the probe to the first reference point and select **Reference value, point 1** to open the stabilizing graph view. Wait for the measurement to stabilize fully.

The stabilization typically takes at least 10–15 minutes.

- a. When the reading has stabilized, press .
- b. Use the arrow buttons to set the value of the reference, and then select **OK** or **Set**.



If you already have the reference and measured values available for your calibration point(s), you can just skip the stabilizing graph view with the  button to get to the view where you can set the reference value. Then replace the automatically filled **Measured value, point 1** and **Measured temperature, point 1** with your actual values.

9. If you want to adjust the measurement in 2 points, place the probe to the second reference point. Then scroll down the **<parameter> adjustment** view and select **Reference value, point 2** to open the stabilizing graph view. Wait for the measurement to stabilize fully.
 - a. When the reading has stabilized, press .
 - b. Use the arrow buttons to set the value of the second reference, and then select **OK** or **Set**.
10. In **<parameter> adjustment** view, check the difference between each reference and measured value. Very large differences may be due to insufficient stabilization time or unsuitable calibration setup.
 - To store the adjustments to the probe, scroll down and select **Activate adjustment > OK**. Confirm by selecting **OK**.
 - To exit without taking the adjustment in use, press  to end calibration.
11. Update the calibration information in **Calibrate / Adjust > Calibration information**. Navigate to the **Calibration information** menu by pressing .
12. Press  to end calibration.

More information

- [Connecting probes to Indigo80 \(page 64\)](#)
- [Adjustment points and requirements \(page 71\)](#)



8.6.3 Restoring factory adjustment with Indigo80 handheld indicator



- Probe connection cable

If needed, you can restore the factory adjustment for your probe's output parameters using the Indigo80 handheld indicator.

Note that restoring the factory adjustment is not necessary before a new adjustment: you can just perform the new adjustment on top of the old adjustment. However, you can select to do the restore procedure if your adjustment fails for some reason, or if you want to return to the original factory adjustment.

- ▶ 1. Connect the probe(s) to the indicator.
2. Open the main menu by pressing .
3. Select **Devices**. If you have more than one device connected to the indicator, make a further selection between the devices.
4. Select **Calibrate / Adjust**.
5. Select the type of adjustment to restore.
For example, select **RH adjustment**.
6. Select **Manual adjustment**.
7. Scroll down and select **Restore factory adjustment > OK**.
8. Confirm by selecting **OK**.
9. Press  to end calibration.

More information

- ▶ [Connecting probes to Indigo80 \(page 64\)](#)

9. Maintenance

9.1 Cleaning the HMP and TMP probes



CAUTION! Do not attempt to clean the sensors under the filter.



Do not spray anything directly on the probe head, since that may deposit impurities on the sensors.

You can clean the probe, probe body, and cable by wiping them with a soft, lint-free cloth moistened with water or a suitable cleaning agent, such as isopropyl alcohol. Do not wipe the filter: wiping the filter may block its pores and/or deposit residue on the filter. If the filter is heavily contaminated, replace it.

When cleaning, follow these precautions:

- Avoid touching the filter. If you need to touch the filter, always wear clean gloves (cotton, rubber or similar material). Keep the filter free of any grease or oil.
- Do not scrape the probe or the probe body.
- Do not immerse the probe or the probe body in liquid to clean them.
- Wipe cleaning agents off the probe, probe body, and the cable after cleaning.

After cleaning the probe, it is recommended to perform sensor purge.

9.2 Cleaning the MMP8 probe



- Instrument air
- Soft, lint-free cloth
- Purified gasoline or heptane liquid
- Isopropyl alcohol



Wear protective eyewear and gloves.

This procedure describes how to clean the MMP8 Moisture in Oil Probe after detaching it from its measurement location. Clean the probe using these instructions before storage, shipping, calibration, or sensor replacement.

Cleaning the probe and its sensor is important to prevent oxidation of the oil on the sensor. Oxidized oil residue on the sensor may lead to extended response times and measurement drift.

- Do not scrape the probe or the probe body.
 - Do not immerse the probe body (the part that contains the M12 connector) in liquid.
- ▶
1. Wipe the probe head with a soft, lint-free cloth to remove any oil on the surface.
 2. Immerse the tip of the probe head in purified gasoline or heptane liquid. Make sure the filter is completely immersed. Move the tip of the probe head in the liquid to clean the filter and the sensor.
 3. With the filter still attached, blow on the probe head with instrument air.
 4. Remove the filter and dry the sensor gently with instrument air. Check that the sensor looks clean. Sensor replacement is recommended for sensors that appear dirty after being cleaned in this manner.
 5. Reattach the filter and tighten it properly (recommended force 5 Nm).
 6. Wipe the probe body, cable, and probe head with a soft, lint-free cloth moistened with isopropyl alcohol.

9.3 Chemical tolerance



Avoid exposing the probe to cleaning agents for unnecessarily long periods of time.

Table 6 Suitability of cleaning agents

| Cleaning Agent | Suitability |
|------------------------|-------------|
| Acetone | Suitable |
| Chlorine disinfectants | Suitable |
| Ethanol | Suitable |
| Heptane | Suitable |
| Isopropyl alcohol | Suitable |

9.4 Changing the probe filter



- New compatible filter
- Clean lint-free gloves



CAUTION! Sensors are easily damaged when the filter is not in place. Handle the probe head carefully.



HMP9 and TMP1 probe models do not have a removable filter.

- ▶ 1. Put on clean gloves before touching the filter.
2. Turn the filter counter-clockwise to loosen it.
3. Remove the filter from the probe head. Be careful not to touch the sensors with the filter.
4. Install a new filter on the probe head. Tighten the filter properly (recommended force 5 Nm).

9.5 Replacing the HUMICAP® sensor



- New HUMICAP® R2 sensor
- New compatible filter
- Clean lint-free gloves
- 11.3 %RH and 75.5 %RH humidity references (using Vaisala HMK15 Humidity Calibrator), or other humidity references of your choice
- Computer with a Microsoft Windows® operating system (64-bit version) and Vaisala Insight PC software installed
- Indigo USB adapter (item code USB2) or USB connection cable (item code 242659)

Follow this procedure to replace a HUMICAP® R2 humidity sensor if it has been damaged, or normal adjustment is not sufficient to restore the humidity measurement accuracy. It is recommended that you replace the filter at the same time. The procedure includes a special 2-point adjustment of humidity measurement using the Insight PC software. This **RH adjustment for new sensor** must be done every time after the HUMICAP® R2 sensor has been replaced.

Of the humidity sensors available in HMP series probes, only HUMICAP® R2 sensors are designed to be replaced by the user. If you need to replace another type of humidity sensor, such as a composite sensor, contact a Vaisala Service Center.



CAUTION! Sensors are easily damaged when the filter is not in place. Handle the probe head carefully.

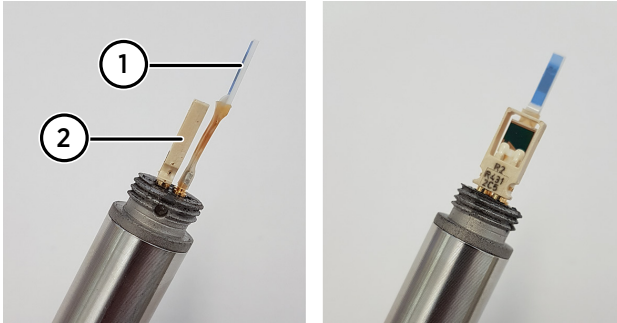


Figure 40 Example: HMP3 probe head with filter removed

- 1 Pt100 temperature sensor
- 2 HUMICAP® R2 humidity sensor

- ▶ 1. Put on clean gloves before touching the filter.
- 2. Turn the filter counter-clockwise to loosen it.
- 3. Remove the filter from the probe head. Be careful not to touch the sensors with the filter.
- 4. There are two sensors under the filter, the HUMICAP® sensor and a temperature sensor. Identify the HUMICAP® sensor and make sure it is of the type that you can replace yourself (temperature sensor not attached to it).
- 5. Pull out the old HUMICAP® sensor and insert the new one.



CAUTION! Handle the new sensor by the plastic frame. Do not touch the sensor element in the middle of the sensor. Do not touch the temperature sensor.

- 6. Open the Insight software on your PC.
- 7. Select **Settings > Advanced mode**.
- 8. Connect the probe to the Insight software.
- 9. Select **⚙ > Calibrate > Yes** to switch the probe to calibration mode.

In calibration mode, the device will not use functions that may interfere with calibration and adjustment.

- 10. Select **RH adjustment for new sensor**.

11. Adjust the 11.3 %RH point (dry end):
 - a. Insert the probe head in the 11.3 %RH reference.
 - b. Wait for the measurement to stabilize fully.
 - c. When the measurement has stabilized, click the **Reference value, point 1** field and enter the RH level of the first reference point (**11 . 3**). Press **ENTER** or click outside the field when done.
 - d. The probe automatically enters the measured temperature value for the calibration point.
12. Adjust the 75.5 %RH point (wet end):
 - a. Insert the probe head in the 75.5 %RH reference.
 - b. Wait for the measurement to stabilize fully.
 - c. When the measurement has stabilized, click the **Reference value, point 2** field and enter the RH level of the second reference point (**75 . 5**). Press **ENTER** or click outside the field when done.
 - d. The probe automatically enters the measured temperature value for the calibration point.
13. To save the adjustment into the device, select **Overwrite factory adjustment**.
14. Remove the probe head from the calibration reference and install a new filter. Tighten the filter properly (recommended force 5 Nm).
15. Select the **Calibration information** tab and update the **Calibration date** and **Calibration text**.
16. Select **Close** to exit the calibration mode.

More information

- [Connecting to Insight software \(page 53\)](#)

10. Troubleshooting

10.1 Problem situations

Table 7 Troubleshooting table

| Problem | Possible cause | Solution |
|--|---|--|
| Measurement output seems incorrect | Installation location is not representative of actual conditions you want to measure | Verify the installation location and relocate the probe if necessary. |
| | Heat conduction along probe head and cable is interfering with measurement accuracy | Follow the installation recommendations for cases when temperature of measured environment differs greatly from ambient. See Installation (page 26) . |
| | Probe is in need of adjustment | Calibrate and adjust the probe. |
| Probe status indicator LED is red | Probe is in error state | Connect the probe to Insight software or an Indigo transmitter and read the error message(s). See Vaisala Insight software (page 53) and Error messages (page 87) . |
| Probe status indicator LED is off even though power is on | Probe model is HMP1, or HMP3/HMP7 with a 0.15-m (0.49-ft) probe connection cable. | To prevent the warming of the indicator LED from causing a slight measurement error, HMP1 probes keep the indicator normally off (even when power is on). If the probe is in error state, the red LED is shown. The same applies to HMP3 and HMP7 probes with a 0.15-m (0.49-ft) probe connection cable. |
| Values of measurement parameters stop changing for a few minutes | Probe is performing a sensor heating function such as sensor purge or waiting for the sensor to cool down | Wait for the function to complete and measurement parameters to be available again. |

10.2 Error messages

Probes can communicate with error messages when they are connected to an Indigo transmitter or Insight software. The messages are categorized according to the severity of the status:

- **Critical errors** are fatal to the operation of the device. It may not be able to respond to communication at all, and will not measure correctly.
- **Errors** prevent normal operation of the device. Depending on the problem, errors may resolve themselves. For example, a completely wet humidity sensor may cause a humidity measurement error.
- **Warnings** do not prevent normal operation but may indicate possible problems.
- **Status** indicates a known state of the device.


| Error message | Description | Recommended action |
|--|--|--|
| Critical errors | | |
| Firmware checksum mismatch [49] | The installed firmware is corrupted. | Contact Vaisala technical support. |
| Device settings corrupted [50] | Parameter memory is corrupted. | |
| Additional configuration settings corrupted [51] | | |
| Sensor coefficients corrupted [52] | | |
| Main configuration settings corrupted [53] | | |
| Factory default settings corrupted [54] | | |
| Non-volatile memory read write failure [57] | Hardware fault. | |
| Errors | | |
| Temperature measurement error [44] | Readings from sensor(s) are missing or out of range. | Inspect probe head and sensors visually. If the probe is completely wet, allow it to dry out. If the sensors are damaged or missing and the error message(s) stay active, contact Vaisala to have the probe repaired. |
| Humidity measurement error [45] | | |
| Humidity sensor failure [46] | | |

| Errors | | |
|--|--|---|
| Capacitance reference error [47] | Hardware fault. | Contact Vaisala technical support. |
| Sensor heater error [212] | | |
| General device failure [994] | High number of measurement errors, capacitance reference errors, or sensor heater errors written in the error log. | |
| Ambient temperature out of range [48] | Probe body is too hot or cold. | Relocate the probe body so that its ambient temperature is within the specified operating range. |
| Supply voltage out of range [55] | Probe supply voltage is too high or low. | Check and correct the supply voltage. |
| Warnings | | |
| Calibration certificate checksum mismatch [58] | Certificate stored in the probe has an invalid checksum. | Contact Vaisala technical support |
| Calibration has expired [353] | This warning is displayed by the calibration reminder functionality if the calibration interval has been exceeded. | Calibrate the probe and update the calibration date information. |
| Supply voltage too low for probe heating [678] | Probe heating is enabled but supply voltage is too low for probe to use it. | This warning is expected when probe heating is enabled and the probe is connected to Insight software using a USB cable. The operating voltage provided by the cable is not sufficient for probe heating. If probe is not connected using a Vaisala USB cable, check the supply voltage. |
| Software restart [679] | The probe has automatically restarted itself. | Check that supply voltage is stable and operating environment is within specification. |
| Unexpected device restart [216] | | |
| Status messages | | |
| Calibration is about to expire [352] | This message is displayed by the calibration reminder functionality. | Calibrate the probe and update the calibration date information. |
| Purge in progress [287] | Sensor purge of the humidity sensor is ongoing. | Wait for sensor purge to complete. |

| Status messages | | |
|--|--|--|
| The readings stay frozen until the sensor cools down [288] | Probe is waiting for its sensors to cool down. | Wait for measurement readings to become available. |

10.3 Restoring factory default settings with Insight software

If needed, you can restore the probe back to its factory default settings using the Insight software. Doing this will also clear any user adjustment and restore the latest adjustment performed by Vaisala.

- ▶ 1. Connect the probe to the Insight software.
2. Select  > **Factory default settings** > **Restore settings**.
3. Wait for the probe to be re-detected.

More information


- ▶ [Connecting to Insight software \(page 53\)](#)

10.4 Restoring factory default settings with Indigo80 handheld indicator



- Probe connection cable

If needed, you can restore the probe back to its factory default settings using the Indigo80 handheld indicator. The user adjustment of the probe and the settings or log files of the indicator itself are not affected.

- ▶ 1. Connect the probe(s) to the indicator.
2. Open the main menu by pressing .
3. Select **Devices**. If you have more than one device connected to the indicator, make a further selection between the devices.
4. Select **Settings**.
5. Scroll down and select **Factory default settings** > **Restore settings** > **OK**.
6. Confirm by selecting **OK**.

More information

- ▶ [Connecting probes to Indigo80 \(page 64\)](#)

11. Technical data

11.1 HMP1 specifications

Table 8 HMP1 measurement performance

| Property | Description/Value |
|--|---|
| Relative humidity | |
| Measurement range | 0-100 %RH |
| Accuracy at +23 °C (+73.4 °F) ^{1) 2)} | ±1.0 %RH (0-90 %RH) |
| Factory calibration uncertainty ³⁾ | ±0.7 %RH (0-40 %RH) ±1 %RH (40-95 %RH) |
| Non-linearity | 0.4 %RH |
| T ₆₃ response time ⁴⁾ | 21 s |
| Sensor | HUMICAP® I |
| Temperature | |
| Measurement range | -40 ... +60 °C (-40 ... +140 °F) |
| Accuracy at +23 °C (+73.4 °F) ^{1) 2)} | ±0.2 °C (±0.36 °F) |
| Factory calibration uncertainty ³⁾ | ±0.1 °C (±0.18 °F) at +23 °C (+73.4 °F) |
| T ₆₃ response time ⁴⁾ | 70 s |

- 1) Defined against calibration reference. Including non-linearity, hysteresis, and repeatability.
- 2) In typical room conditions.
- 3) Defined as ±2 standard deviation limits. Small variations possible; see calibration certificate.
- 4) In still air.

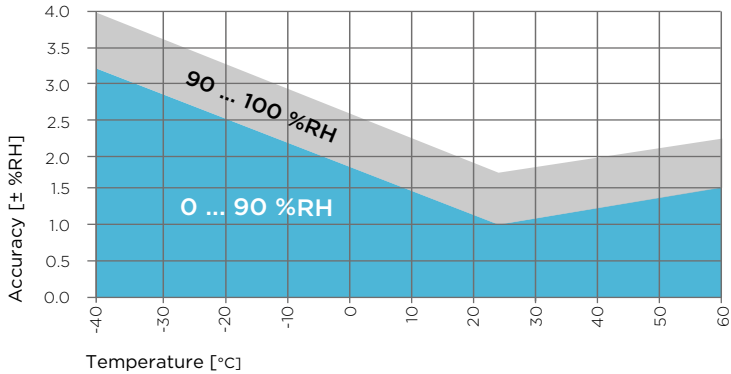


Figure 41 HMP1 humidity measurement accuracy as a function of temperature

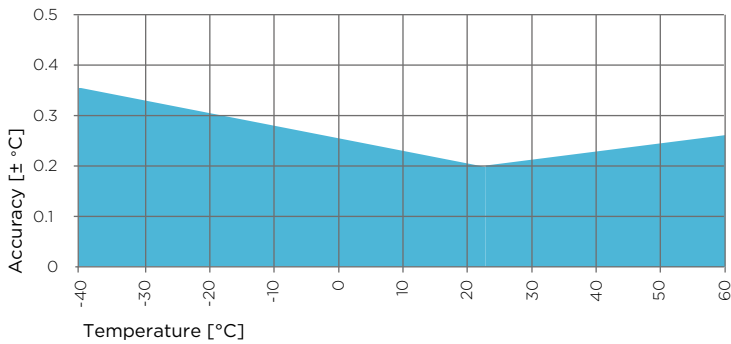


Figure 42 HMP1 temperature measurement accuracy over full range

Table 9 HMP1 operating environment

| Property | Description/Value |
|-------------------------|--|
| Operating temperature | -40 ... +60 °C (-40 ... +140 °F) |
| Storage temperature | -40 ... +60 °C (-40 ... +140 °F) |
| Measurement environment | For air, nitrogen, hydrogen, argon, helium, and oxygen ¹⁾ |
| IP rating | IP50: Limited protection against dust. |

1) Consult Vaisala if other chemicals are present. Consider safety regulations with flammable gases.

Table 10 HMP1 inputs and outputs

| Property | Description/Value |
|---------------------|---------------------------|
| Operating voltage | 15–30 V DC |
| Current consumption | 2 mA typical, 200 mA max. |
| Digital output | RS-485, non-isolated |
| Protocol | Modbus RTU |

Table 11 HMP1 output parameters

| Output parameter name and unit | |
|--|---|
| Absolute humidity (g/m ³) | Relative humidity (%RH) |
| Absolute humidity at NTP (g/m ³) | Relative humidity (dew/frost) (%RH) |
| Dew point temperature (°C) | Temperature (°C) |
| Dew/frost point temperature (°C) | Water concentration (ppm _v) |
| Dew/frost point temperature at 1 atm (°C) | Water concentration (wet basis) (vol-%) |
| Dew point temperature at 1 atm (°C) | Water mass fraction (ppm _w) |
| Dew point temperature difference (°C) | Water vapor pressure (hPa) |
| Enthalpy (kJ/kg) | Water vapor saturation pressure (hPa) |
| Mixing ratio (g/kg) | Wet-bulb temperature (°C) |

Table 12 HMP1 compliance

| Property | Value/Description |
|-------------------------------------|---|
| EU directives and regulations | EMC Directive (2014/30/EU) RoHS Directive (2011/65/EU) amended by 2015/863 |
| Electromagnetic compatibility (EMC) | EN 61326-1, industrial environment |
| Compliance marks | CE, China RoHS, RCM |

Table 13 HMP1 mechanical specifications

| Property | Description/Value |
|------------------|------------------------|
| Connector | M12 5-pin A-coded male |
| Weight | 38 g (1.34 oz) |
| Materials | |

| Property | Description/Value |
|------------|-------------------|
| Probe | AISI 316L |
| Probe body | PBT |

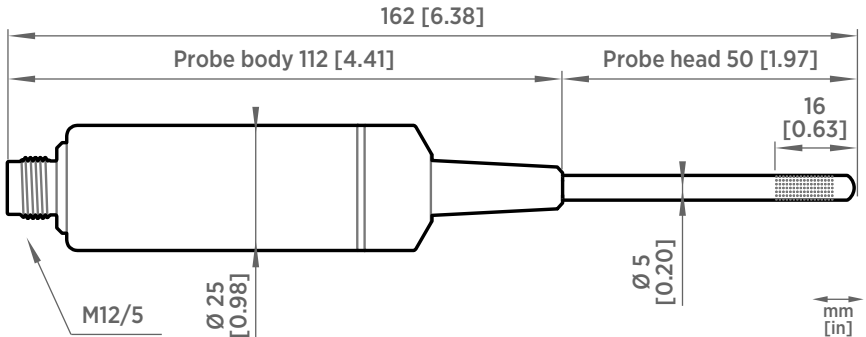


Figure 43 HMP1 probe dimensions

11.2 HMP3 specifications

Table 14 HMP3 measurement performance

| Property | Description/Value |
|---|--|
| Relative humidity | |
| Measurement range | 0–100 %RH, at max. +95 °C (203 °F) T _d |
| Accuracy at +23 °C (+73.4 °F) ¹⁾ | ±0.8 %RH (0–90 %RH) |
| Factory calibration uncertainty ²⁾ | ±0.5 %RH (0–40 %RH) ±0.8 %RH (40–95 %RH) |
| T ₆₃ response time | 15 s |
| Sensor options | HUMICAP® R2 HUMICAP® R2C ³⁾ HUMICAP® 180VC ^{3) 4)} |
| Temperature | |
| Sensor | Pt100 RTD Class F0.1 IEC 60751 |
| Measurement range | –40 ... +120 °C (–40 ... +248 °F) |
| Accuracy ^{1) 5)} | ±0.1 °C (±0.18 °F) |

| Property | Description/Value |
|---|---|
| Factory calibration uncertainty ²⁾ | ±0.1 °C (±0.18 °F) at +23 °C (+73.4 °F) |

- 1) Defined against calibration reference. Including non-linearity, hysteresis, and repeatability.
- 2) Defined as ±2 standard deviation limits. Small variations possible; see calibration certificate.
- 3) Sensor purge feature available with this sensor.
- 4) H₂O₂ resistant. With HUMICAP® 180VC sensor, accuracy is not specified below -20 °C (-4 °F) operating temperature.
- 5) Exposing temperature sensor to temperatures outside -20 ... +150 °C (-4 ... +302 °F) may cause permanent additional deviation of ±0.1 °C (0.18 °F)

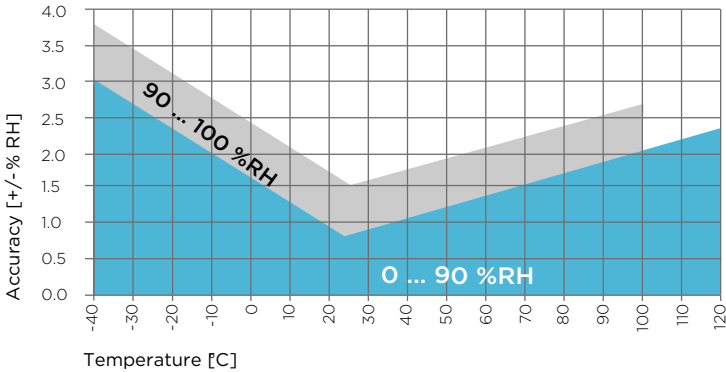


Figure 44 HMP3 humidity measurement accuracy as a function of temperature

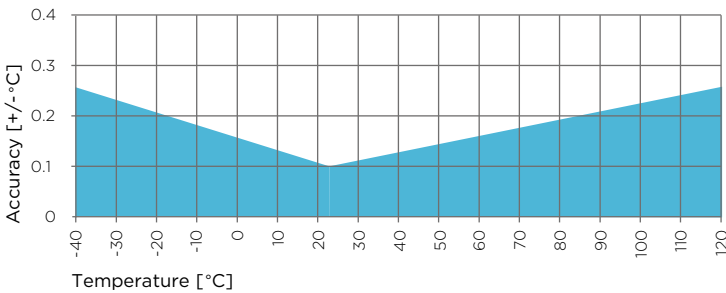


Figure 45 HMP3 temperature measurement accuracy over full range

Table 15 HMP3 operating environment

| Property | Description/Value |
|-------------------------------------|----------------------------------|
| Operating temperature of probe body | -40 ... +80 °C (-40 ... +176 °F) |

| Property | Description/Value |
|-------------------------------------|--|
| Operating temperature of probe head | -40 ... +120 °C (-40 ... +248 °F) |
| Operating humidity of probe head | Max. +100 °C (212 °F) T _d |
| Storage temperature | -40 ... +80 °C (-40 ... +176 °F) |
| Operating environment | Suitable for outdoor use |
| Measurement environment | For air, nitrogen, hydrogen, argon, helium, and oxygen ¹⁾ |
| IP rating of probe body | IP66: Dust-tight. Protected from powerful water jets from any direction. |

1) Consult Vaisala if other chemicals are present. Consider safety regulations with flammable gases.

Table 16 HMP3 inputs and outputs

| Property | Description/Value |
|---------------------|----------------------------|
| Operating voltage | 15–30 V DC |
| Current consumption | 10 mA typical, 500 mA max. |
| Digital output | RS-485, non-isolated |
| Protocols | Modbus RTU |

Table 17 HMP3 output parameters

| Output parameter name and unit | |
|--|---|
| Absolute humidity (g/m ³) | Relative humidity (%RH) |
| Absolute humidity at NTP (g/m ³) | Relative humidity (dew/frost) (%RH) |
| Dew point temperature (°C) | Temperature (°C) |
| Dew/frost point temperature (°C) | Water concentration (ppm _v) |
| Dew/frost point temperature at 1 atm (°C) | Water concentration (wet basis) (vol-%) |
| Dew point temperature at 1 atm (°C) | Water mass fraction (ppm _w) |
| Dew point temperature difference (°C) | Water vapor pressure (hPa) |
| Enthalpy (kJ/kg) | Water vapor saturation pressure (hPa) |
| Mixing ratio (g/kg) | Wet-bulb temperature (°C) |

Table 18 HMP3 compliance

| Property | Value/Description |
|-------------------------------------|---|
| EU directives and regulations | EMC Directive (2014/30/EU) RoHS Directive (2011/65/EU) amended by 2015/863 |
| Electromagnetic compatibility (EMC) | EN 61326-1, industrial environment |
| Type approvals | DNV GL certificate no. TAA00002YT |
| Compliance marks | CE, China RoHS, RCM |

Table 19 HMP3 mechanical specifications

| Property | Description/Value |
|---------------------------|--|
| Connector | M12 5-pin A-coded male |
| Weight (with a 2-m cable) | 302 g (10.65 oz) |
| Probe cable length | 0.15 m (0.49 ft), 2 m (6.56 ft), 5 m (16.40 ft) or 10 m (32.80 ft) |
| Materials | |
| Probe | AISI 316L |
| Probe body | AISI 316L |
| Cable jacket | FEP |

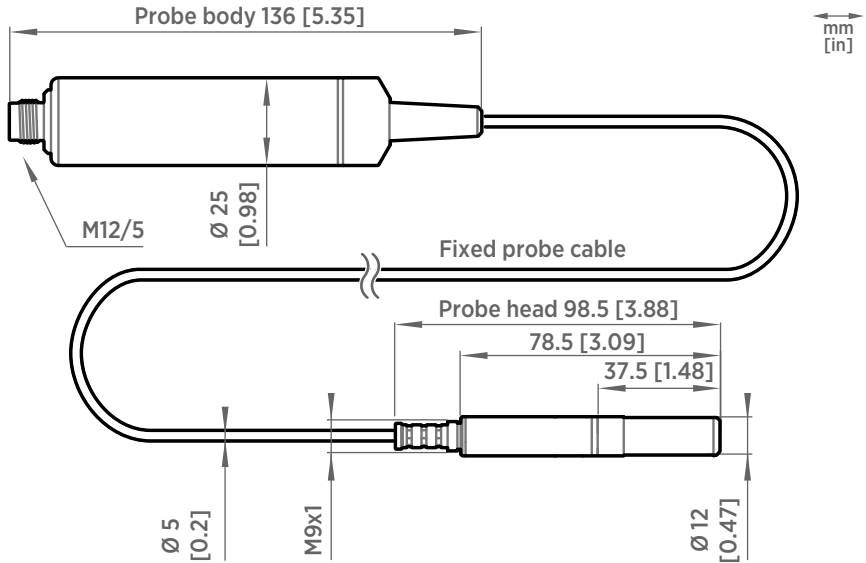


Figure 46 HMP3 probe dimensions

11.3 HMP4 specifications

Table 20 HMP4 measurement performance

| Property | Description/Value |
|---|---|
| Relative humidity | |
| Measurement range | 0–100 %RH, at max. +95 °C (203 °F) T_d |
| Accuracy at +23 °C (+73.4 °F) ¹⁾ | ±0.8 %RH (0–90 %RH) |
| Factory calibration uncertainty ²⁾ | ±0.5 %RH (0–40 %RH) ±0.8 %RH (40–95 %RH) |
| T_{63} response time | 15 s |
| Sensor options | HUMICAP® R2 HUMICAP® R2C ³⁾ |
| Temperature | |
| Measurement range | –70 ... +180 °C (–94 ... +356 °F) |
| Accuracy ^{1) 4)} | ±0.1 °C (±0.18 °F) |

| Property | Description/Value |
|---|---|
| Factory calibration uncertainty ²⁾ | ±0.1 °C (±0.18 °F) at +23 °C (+73.4 °F) |
| Sensor | Pt100 RTD Class F0.1 IEC 60751 |

- 1) Defined against calibration reference. Including non-linearity, hysteresis, and repeatability.
- 2) Defined as ±2 standard deviation limits. Small variations possible; see calibration certificate.
- 3) Sensor purge feature available with this sensor.
- 4) Exposing temperature sensor to temperatures outside -20 ... +150 °C (-4 ... +302 °F) may cause permanent additional deviation of ±0.1 °C (0.18 °F)

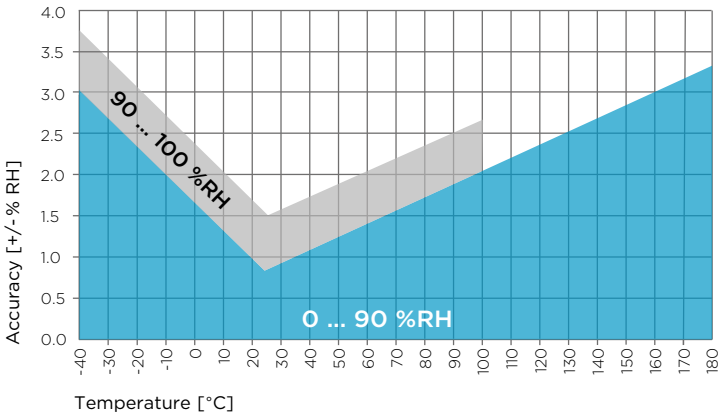


Figure 47 HMP4 humidity measurement accuracy as a function of temperature

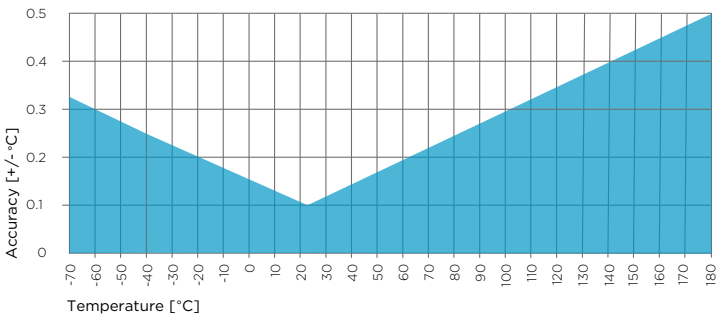


Figure 48 HMP4 temperature measurement accuracy over full range

Table 21 HMP4 operating environment

| Property | Description/Value |
|-------------------------------------|--|
| Operating temperature of probe body | -40 ... +80 °C (-40 ... +176 °F) |
| Operating temperature of probe head | -70 ... +180 °C (-94 ... +356 °F) |
| Operating humidity of probe head | Max. +100 °C (212 °F) T _d |
| Storage temperature | -40 ... +80 °C (-40 ... +176 °F) |
| Operational pressure | < 100 bar |
| Operating environment | Suitable for outdoor use |
| Measurement environment | For air, nitrogen, hydrogen, argon, helium, oxygen, and vacuum ¹⁾ |
| IP rating of probe body | IP66: Dust-tight. Protected from powerful water jets from any direction. |

1) Consult Vaisala if other chemicals are present. Consider safety regulations with flammable gases.

Table 22 HMP4 inputs and outputs

| Property | Description/Value |
|---------------------|----------------------------|
| Operating voltage | 15–30 V DC |
| Current consumption | 10 mA typical, 500 mA max. |
| Digital output | RS-485, non-isolated |
| Protocols | Modbus RTU |

Table 23 HMP4 output parameters

| Output parameter name and unit | |
|--|---|
| Absolute humidity (g/m ³) | Relative humidity (%RH) |
| Absolute humidity at NTP (g/m ³) | Relative humidity (dew/frost) (%RH) |
| Dew point temperature (°C) | Temperature (°C) |
| Dew/frost point temperature (°C) | Water concentration (ppm _v) |
| Dew/frost point temperature at 1 atm (°C) | Water concentration (wet basis) (vol-%) |
| Dew point temperature at 1 atm (°C) | Water mass fraction (ppm _w) |
| Dew point temperature difference (°C) | Water vapor pressure (hPa) |
| Enthalpy (kJ/kg) | Water vapor saturation pressure (hPa) |

| Output parameter name and unit | |
|--------------------------------|---------------------------|
| Mixing ratio (g/kg) | Wet-bulb temperature (°C) |

Table 24 HMP4 compliance

| Property | Value/Description |
|-------------------------------------|---|
| EU directives and regulations | EMC Directive (2014/30/EU) RoHS Directive (2011/65/EU) amended by 2015/863 |
| Electromagnetic compatibility (EMC) | EN 61326-1, industrial environment |
| Type approvals | DNV GL certificate no. TAA00002YT |
| Compliance marks | CE, China RoHS, RCM |

Table 25 HMP4 mechanical specifications

| Property | Description/Value |
|---------------------------|------------------------|
| Connector | M12 5-pin A-coded male |
| Fitting body | M22×1.5 or NPT1/2" |
| Weight (with a 2-m cable) | 530 g (18.7 oz) |
| Probe cable length | 2 m (6.56 ft) |
| Materials | |
| Probe | AISI 316 |
| Probe body | AISI 316 |
| Cable jacket | FEP |

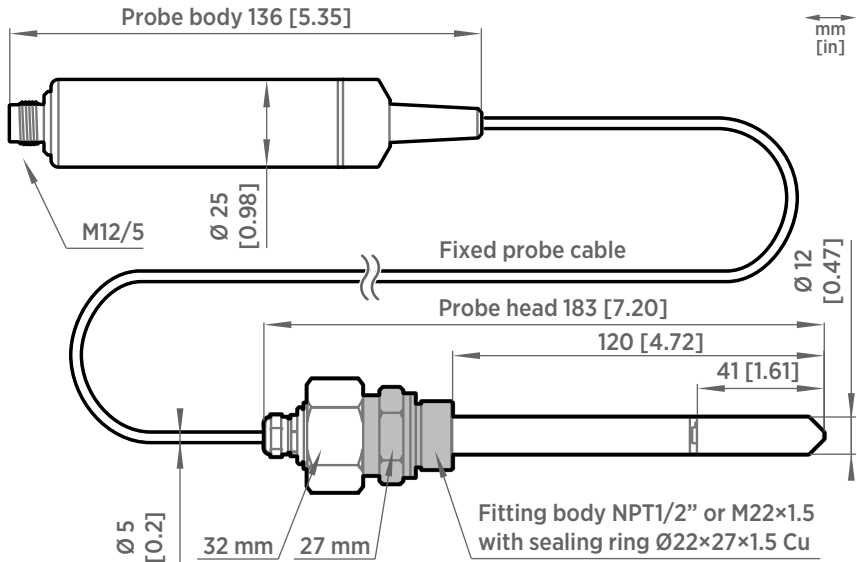


Figure 49 HMP4 probe dimensions

11.4 HMP5 specifications

Table 26 HMP5 measurement performance

| Property | Description/Value |
|--|---|
| Relative humidity | |
| Measurement range | 0–100 %RH, at max. +95 °C (203 °F) T_d |
| Accuracy at +23 °C (+73.4 °F) ¹⁾ | ±0.8 %RH (0–90 %RH) |
| Factory calibration uncertainty ²⁾ | ±0.5 %RH (0–40 %RH) ±0.8 %RH (40–95 %RH) |
| T_{63} response time | 15 s |
| Sensor options | HUMICAP® R2 HUMICAP® R2C ³⁾ |
| Temperature | |
| Measurement range | –70 ... +180 °C (–94 ... +356 °F) |
| Accuracy at +23 °C (+73.4 °F) ^{1) 4)} | ±0.1 °C (±0.18 °F) |

| Property | Description/Value |
|---|---|
| Factory calibration uncertainty ²⁾ | ±0.1 °C (±0.18 °F) at +23 °C (+73.4 °F) |
| Sensor | Pt100 RTD Class F0.1 IEC 60751 |

- 1) Defined against calibration reference. Including non-linearity, hysteresis, and repeatability.
- 2) Defined as ±2 standard deviation limits. Small variations possible; see calibration certificate.
- 3) Sensor purge feature available with this sensor.
- 4) Exposing temperature sensor to temperatures outside -20 ... +150 °C (-4 ... +302 °F) may cause permanent additional deviation of ±0.1 °C (0.18 °F)

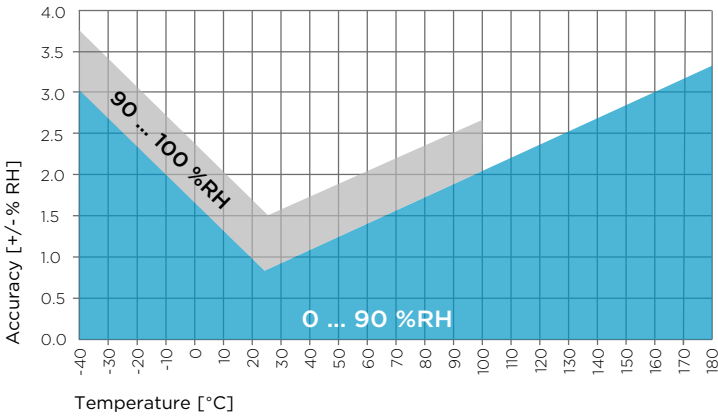


Figure 50 HMP5 humidity measurement accuracy as a function of temperature

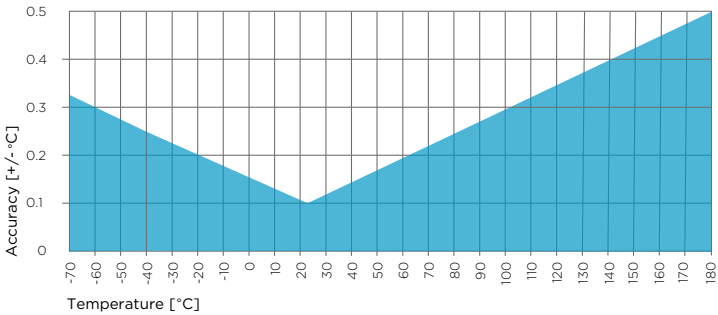


Figure 51 HMP5 temperature measurement accuracy over full range

Table 27 HMP5 operating environment

| Property | Description/Value |
|-------------------------------------|--|
| Operating temperature of probe body | -40 ... +80 °C (-40 ... +176 °F) |
| Operating temperature of probe head | -70 ... +180 °C (-94 ... +356 °F) |
| Operating humidity of probe head | Max. +100 °C (212 °F) T _d |
| Storage temperature | -40 ... +80 °C (-40 ... +176 °F) |
| Operating environment | Suitable for outdoor use |
| IP rating of probe body | IP66: Dust-tight. Protected from powerful water jets from any direction. |

Table 28 HMP5 inputs and outputs

| Property | Description/Value |
|---------------------|----------------------------|
| Operating voltage | 15–30 V DC |
| Current consumption | 10 mA typical, 500 mA max. |
| Digital output | RS-485, non-isolated |
| Protocols | Modbus RTU |

Table 29 HMP5 output parameters

| Output parameter name and unit | |
|--|---|
| Absolute humidity (g/m ³) | Relative humidity (%RH) |
| Absolute humidity at NTP (g/m ³) | Relative humidity (dew/frost) (%RH) |
| Dew point temperature (°C) | Temperature (°C) |
| Dew/frost point temperature (°C) | Water concentration (ppm _v) |
| Dew/frost point temperature at 1 atm (°C) | Water concentration (wet basis) (vol-%) |
| Dew point temperature at 1 atm (°C) | Water mass fraction (ppm _w) |
| Dew point temperature difference (°C) | Water vapor pressure (hPa) |
| Enthalpy (kJ/kg) | Water vapor saturation pressure (hPa) |
| Mixing ratio (g/kg) | Wet-bulb temperature (°C) |

Table 30 HMP5 compliance

| Property | Value/Description |
|-------------------------------------|---|
| EU directives and regulations | EMC Directive (2014/30/EU) RoHS Directive (2011/65/EU) amended by 2015/863 |
| Electromagnetic compatibility (EMC) | EN 61326-1, industrial environment |
| Type approvals | DNV GL certificate no. TAA00002YT |
| Compliance marks | CE, China RoHS, RCM |

Table 31 HMP5 mechanical specifications

| Property | Description/Value |
|---------------------------|---------------------------------|
| Connector | M12 5-pin A-coded male |
| Weight (with a 2-m cable) | 436 g (15.37 oz) |
| Probe cable length | 2 m (6.56 ft) or 10 m (32.8 ft) |
| Materials | |
| Probe | AISI 316L |
| Probe body | AISI 316L |
| Cable jacket | FEP |

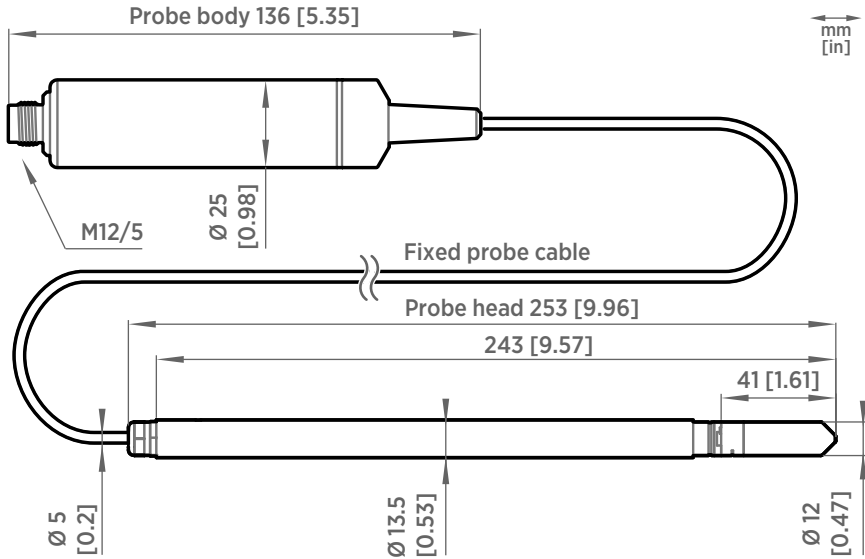


Figure 52 HMP5 probe dimensions

11.5 HMP7 specifications

Table 32 HMP7 measurement performance

| Property | Description/Value |
|---|--|
| Relative humidity | |
| Measurement range | 0–100 %RH, at max. +95 °C (203 °F) T_d |
| Accuracy at +23 °C (+73.4 °F) ¹⁾ | ±0.8 %RH (0–90 %RH) |
| Factory calibration uncertainty ²⁾ | ±0.5 %RH (0–40 %RH) ±0.8 %RH (40–95 %RH) |
| T_{63} response time | 15 s |
| Sensor options | HUMICAP® R2 HUMICAP® R2C ³⁾ HUMICAP® 180VC ^{3) 4)} |
| Temperature | |
| Measurement range | –70 ... +180 °C (–94 ... +356 °F) |

| Property | Description/Value |
|--|---|
| Accuracy at +23 °C (+73.4 °F) ^{1) 5)} | ±0.1 °C (±0.18 °F) |
| Factory calibration uncertainty ²⁾ | ±0.1 °C (±0.18 °F) at +23 °C (+73.4 °F) |
| Sensor | Pt100 RTD Class F0.1 IEC 60751 |

- 1) Defined against calibration reference. Including non-linearity, hysteresis, and repeatability.
- 2) Defined as ±2 standard deviation limits. Small variations possible; see calibration certificate.
- 3) Sensor purge feature available with this sensor.
- 4) H₂O₂ resistant. With HUMICAP® 180VC sensor, accuracy is not specified below -20 °C (-4 °F) operating temperature.
- 5) Exposing temperature sensor to temperatures outside -20 ... +150 °C (-4 ... +302 °F) may cause permanent additional deviation of ±0.1 °C (0.18 °F)

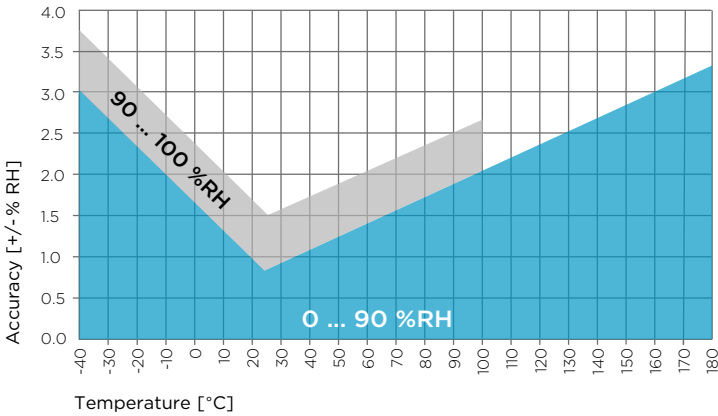


Figure 53 HMP7 humidity measurement accuracy as a function of temperature

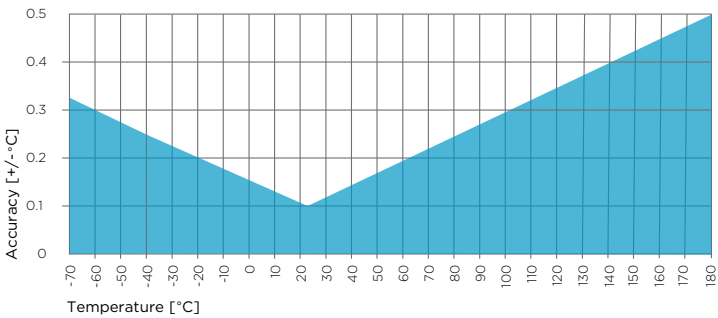


Figure 54 HMP7 temperature measurement accuracy over full range

Table 33 HMP7 operating environment

| Property | Description/Value |
|-------------------------------------|--|
| Operating temperature of probe body | -40 ... +80 °C (-40 ... +176 °F) |
| Operating temperature of probe head | -70 ... +180 °C (-94 ... +356 °F) |
| Operating humidity of probe head | Max. +100 °C (212 °F) T _d |
| Storage temperature | -40 ... +80 °C (-40 ... +176 °F) |
| Operational pressure | < 10 bar |
| Operating environment | Suitable for outdoor use |
| Measurement environment | For air, nitrogen, hydrogen, argon, helium, oxygen, and vacuum ¹⁾ |
| IP rating of probe body | IP66: Dust-tight. Protected from powerful water jets from any direction. |

1) Consult Vaisala if other chemicals are present. Consider safety regulations with flammable gases.

Table 34 HMP7 inputs and outputs

| Property | Description/Value |
|---------------------|----------------------------|
| Operating voltage | 18–30 V DC |
| Current consumption | 10 mA typical, 500 mA max. |
| Digital output | RS-485, non-isolated |
| Protocols | Modbus RTU |

Table 35 HMP7 output parameters

| Output parameter name and unit | |
|--|---|
| Absolute humidity (g/m ³) | Relative humidity (%RH) |
| Absolute humidity at NTP (g/m ³) | Relative humidity (dew/frost) (%RH) |
| Dew point temperature (°C) | Temperature (°C) |
| Dew/frost point temperature (°C) | Water concentration (ppm _v) |
| Dew/frost point temperature at 1 atm (°C) | Water concentration (wet basis) (vol-%) |
| Dew point temperature at 1 atm (°C) | Water mass fraction (ppm _w) |
| Dew point temperature difference (°C) | Water vapor pressure (hPa) |
| Enthalpy (kJ/kg) | Water vapor saturation pressure (hPa) |

| Output parameter name and unit | |
|--------------------------------|---------------------------|
| Mixing ratio (g/kg) | Wet-bulb temperature (°C) |

Table 36 HMP7 compliance

| Property | Value/Description |
|-------------------------------------|---|
| EU directives and regulations | EMC Directive (2014/30/EU) RoHS Directive (2011/65/EU) amended by 2015/863 |
| Electromagnetic compatibility (EMC) | EN 61326-1, industrial environment |
| Type approvals | DNV GL certificate no. TAA00002YT |
| Compliance marks | CE, China RoHS, RCM |

Table 37 HMP7 mechanical specifications

| Property | Description/Value |
|---------------------------|--|
| Connector | M12 5-pin A-coded male |
| Weight (with a 2-m cable) | 310 g (10.9 oz) |
| Probe cable length | 0.15 m (0.49 ft), 2 m (6.56 ft) or 10 m (32.80 ft) |
| Materials | |
| Probe | AISI 316L |
| Probe body | AISI 316L |
| Cable jacket | FEP |

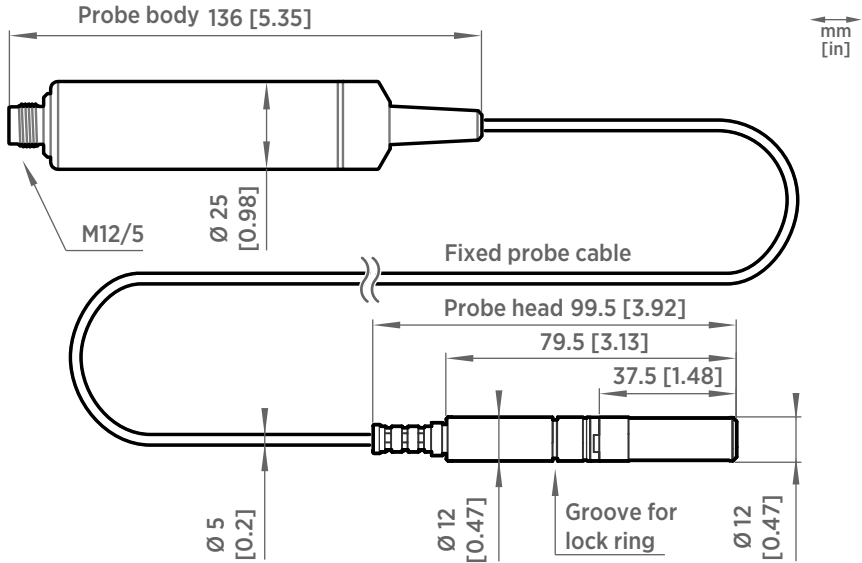


Figure 55 HMP7 probe dimensions

11.6 HMP8 specifications

Table 38 HMP8 measurement performance

| Property | Description/Value |
|--|---|
| Relative humidity | |
| Measurement range | 0–100 %RH, at max. +95 °C (203 °F) T_d |
| Accuracy at +23 °C (+73.4 °F) ¹⁾ | ±0.8 %RH (0–90 %RH) |
| Factory calibration uncertainty ²⁾ | ±0.5 %RH (0–40 %RH) ±0.8 %RH (40–95 %RH) |
| T_{63} response time | 15 s |
| Sensor options | HUMICAP® R2 HUMICAP® R2C ³⁾ |
| Temperature | |
| Measurement range | –70 ... +180 °C (–94 ... +356 °F) |
| Accuracy at +23 °C (+73.4 °F) ^{1) 4)} | ±0.1 °C (±0.18 °F) |

| Property | Description/Value |
|---|---|
| Factory calibration uncertainty ²⁾ | $\pm 0.1 \text{ }^\circ\text{C}$ ($\pm 0.18 \text{ }^\circ\text{F}$) at $+23 \text{ }^\circ\text{C}$ ($+73.4 \text{ }^\circ\text{F}$) |
| Sensor | Pt100 RTD Class F0.1 IEC 60751 |

- 1) Defined against calibration reference. Including non-linearity, hysteresis, and repeatability.
- 2) Defined as ± 2 standard deviation limits. Small variations possible; see calibration certificate.
- 3) Sensor purge feature available with this sensor.
- 4) Exposing temperature sensor to temperatures outside $-20 \dots +150 \text{ }^\circ\text{C}$ ($-4 \dots +302 \text{ }^\circ\text{F}$) may cause permanent additional deviation of $\pm 0.1 \text{ }^\circ\text{C}$ ($0.18 \text{ }^\circ\text{F}$).

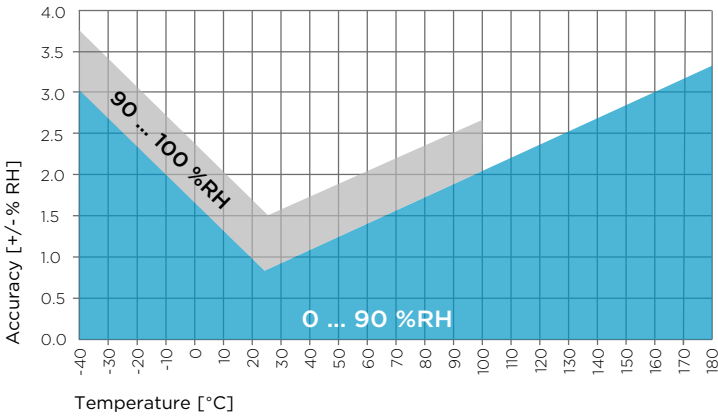


Figure 56 HMP8 humidity measurement accuracy as a function of temperature

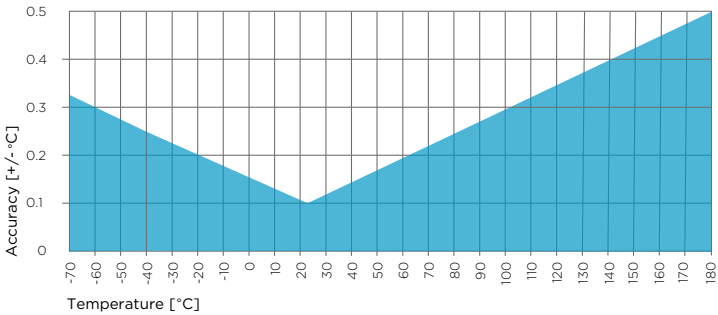


Figure 57 HMP8 temperature measurement accuracy over full range

Table 39 HMP8 operating environment

| Property | Description/Value |
|-------------------------------------|--|
| Operating temperature of probe body | -40 ... +80 °C (-40 ... +176 °F) |
| Operating temperature of probe head | -70 ... +180 °C (-94 ... +356 °F) |
| Operating humidity of probe head | Max. +100 °C (212 °F) T _d |
| Storage temperature | -40 ... +80 °C (-40 ... +176 °F) |
| Operational pressure | < 40 bar |
| Operating environment | Suitable for outdoor use |
| Measurement environment | For air, nitrogen, hydrogen, argon, helium, oxygen, and vacuum ¹⁾ |
| IP rating of probe body | IP66: Dust-tight. Protected from powerful water jets from any direction. |

1) Consult Vaisala if other chemicals are present. Consider safety regulations with flammable gases.

Table 40 HMP8 inputs and outputs

| Property | Description/Value |
|---------------------|----------------------------|
| Operating voltage | 15–30 V DC |
| Current consumption | 10 mA typical, 500 mA max. |
| Digital output | RS-485, non-isolated |
| Protocols | Modbus RTU |

Table 41 HMP8 output parameters

| Output parameter name and unit | |
|--|---|
| Absolute humidity (g/m ³) | Relative humidity (%RH) |
| Absolute humidity at NTP (g/m ³) | Relative humidity (dew/frost) (%RH) |
| Dew point temperature (°C) | Temperature (°C) |
| Dew/frost point temperature (°C) | Water concentration (ppm _v) |
| Dew/frost point temperature at 1 atm (°C) | Water concentration (wet basis) (vol-%) |
| Dew point temperature at 1 atm (°C) | Water mass fraction (ppm _w) |
| Dew point temperature difference (°C) | Water vapor pressure (hPa) |
| Enthalpy (kJ/kg) | Water vapor saturation pressure (hPa) |

| Output parameter name and unit | |
|--------------------------------|---------------------------|
| Mixing ratio (g/kg) | Wet-bulb temperature (°C) |

Table 42 HMP8 compliance

| Property | Value/Description |
|-------------------------------------|---|
| EU directives and regulations | EMC Directive (2014/30/EU) RoHS Directive (2011/65/EU) amended by 2015/863 |
| Electromagnetic compatibility (EMC) | EN 61326-1, industrial environment |
| Type approvals | DNV GL certificate no. TAA00002YT |
| Compliance marks | CE, China RoHS, RCM |

Table 43 HMP8 mechanical specifications

| Property | Description/Value |
|---------------------------|---------------------------------------|
| Connector | M12 5-pin A-coded male |
| Probe fitting | ISO1/2" and NPT1/2" fittings included |
| Weight (with a 2-m cable) | 512 g (18.1 oz) |
| Probe cable length | 2 m (6.56 ft) or 10 m (32.80 ft) |
| Materials | |
| Probe | AISI 316L |
| Probe body | AISI 316L |
| Cable jacket | FEP |

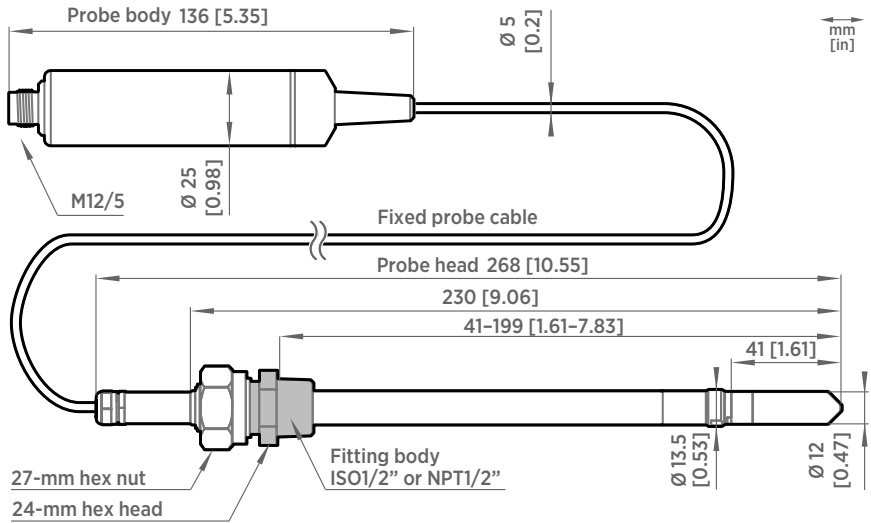


Figure 58 HMP8 probe dimensions

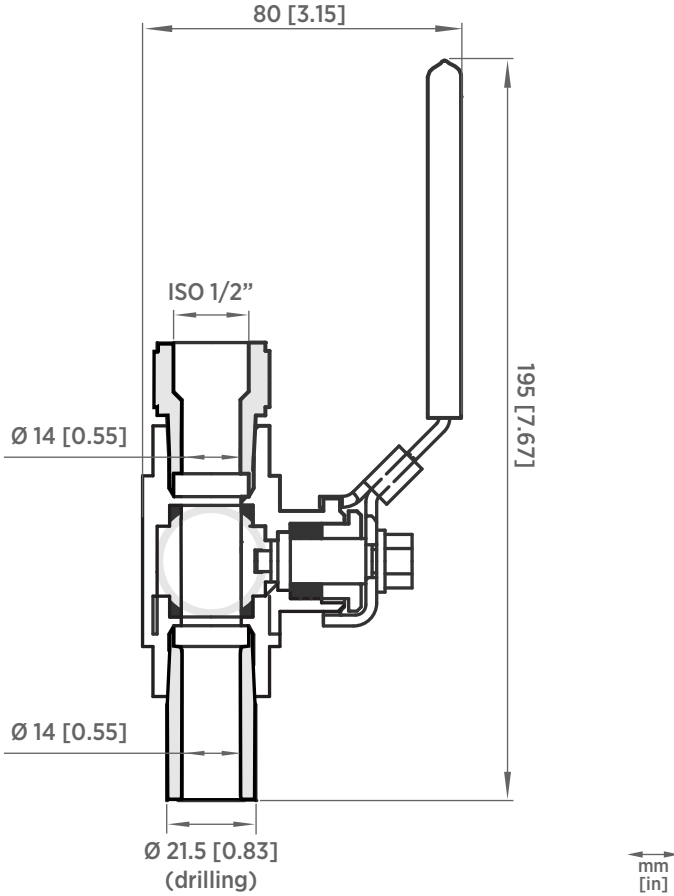


Figure 59 Optional ball valve kit dimensions

11.7 HMP9 specifications

Table 44 HMP9 measurement performance

| Property | Description/Value |
|---|---|
| Relative humidity | |
| Measurement range | 0-100 %RH, at max. +95 °C (203 °F) T _d |
| Accuracy at +23 °C (+73.4 °F) ¹⁾ | ±0.8 %RH (0-90 %RH) |

| Property | Description/Value |
|---|---|
| Factory calibration uncertainty ²⁾ | ±0.7 %RH (0–40 %RH) ±1 %RH (40–95 %RH) |
| Non-linearity | 0.4 %RH |
| T ₆₃ response time ³⁾ | 15 s |
| Sensor | HUMICAP® I |
| Temperature | |
| Measurement range | –40 ... +120 °C (–40 ... +248 °F) |
| Accuracy at +23 °C (+73.4 °F) ¹⁾ | ±0.1 °C (±0.18 °F) |
| Factory calibration uncertainty ²⁾ | ±0.1 °C (±0.18 °F) at +23 °C (+73.4 °F) |
| T ₆₃ response time ³⁾ | 70 s |

- 1) Defined against calibration reference. Including non-linearity, hysteresis, and repeatability.
- 2) Defined as ±2 standard deviation limits. Small variations possible; see calibration certificate.
- 3) In still air.

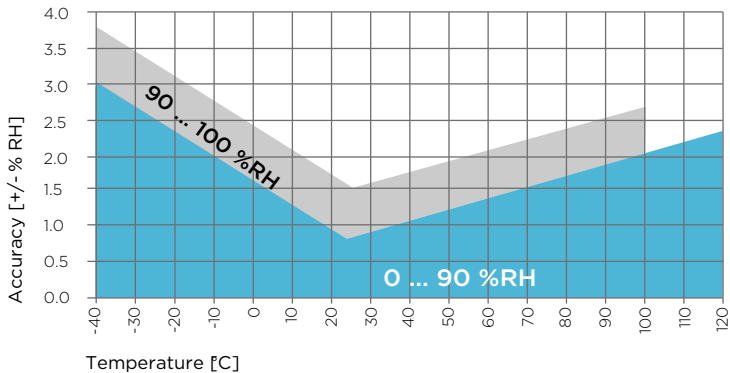


Figure 60 HMP9 humidity measurement accuracy as a function of temperature

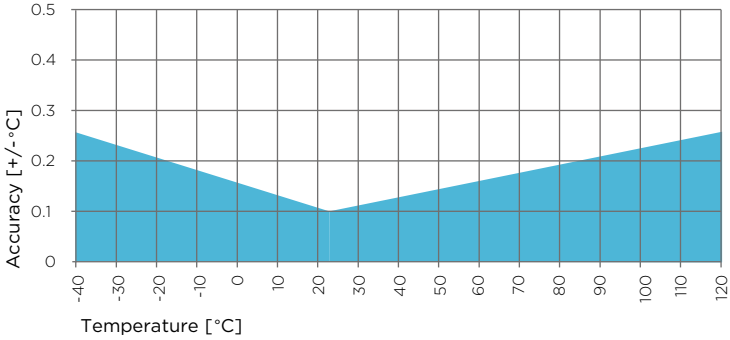


Figure 61 HMP9 temperature measurement accuracy over full range

Table 45 HMP9 operating environment

| Property | Description/Value |
|-------------------------------------|--|
| Operating temperature of probe body | -40 ... +60 °C (-40 ... +140 °F) |
| Operating temperature of probe head | -40 ... +120 °C (-40 ... +248 °F) |
| Operating humidity of probe head | Max. +100 °C (212 °F) T _d |
| Storage temperature | -40 ... +60 °C (-40 ... +140 °F) |
| Operating environment | Suitable for outdoor use when protected from rain |
| Measurement environment | For air, nitrogen, hydrogen, argon, helium, and oxygen ¹⁾ |
| IP rating of probe body | IP65: Dust-tight. Protected from water jets from any direction. |

1) Consult Vaisala if other chemicals are present. Consider safety regulations with flammable gases.

Table 46 HMP9 inputs and outputs

| Property | Description/Value |
|-------------------------|---------------------------|
| Operating voltage | 15–30 V DC |
| Current consumption | 5 mA typical, 400 mA max. |
| Digital output | RS-485, non-isolated |
| Default serial settings | 19200 bps N 8 2 |
| Protocol | Modbus RTU |

Table 47 HMP9 output parameters

| Output parameter name and unit | |
|--|---|
| Absolute humidity (g/m ³) | Relative humidity (%RH) |
| Absolute humidity at NTP (g/m ³) | Relative humidity (dew/frost) (%RH) |
| Dew point temperature (°C) | Temperature (°C) |
| Dew/frost point temperature (°C) | Water concentration (ppm _v) |
| Dew/frost point temperature at 1 atm (°C) | Water concentration (wet basis) (vol-%) |
| Dew point temperature at 1 atm (°C) | Water mass fraction (ppm _w) |
| Dew point temperature difference (°C) | Water vapor pressure (hPa) |
| Enthalpy (kJ/kg) | Water vapor saturation pressure (hPa) |
| Mixing ratio (g/kg) | Wet-bulb temperature (°C) |

Table 48 HMP9 compliance

| Property | Value/Description |
|-------------------------------------|---|
| EU directives and regulations | EMC Directive (2014/30/EU) RoHS Directive (2011/65/EU) amended by 2015/863 |
| Electromagnetic compatibility (EMC) | EN 61326-1, industrial environment |
| Compliance marks | CE, China RoHS, RCM |

Table 49 HMP9 mechanical specifications

| Property | Description/Value |
|---------------------------|------------------------|
| Connector | M12 5-pin A-coded male |
| Weight (with a 2-m cable) | 68 g (2.40 oz) |
| Probe cable length | 2 m (6.56 ft) |
| Materials | |
| Probe | AISI 316L |
| Probe body | PBT |
| Cable overmolds | FEP |

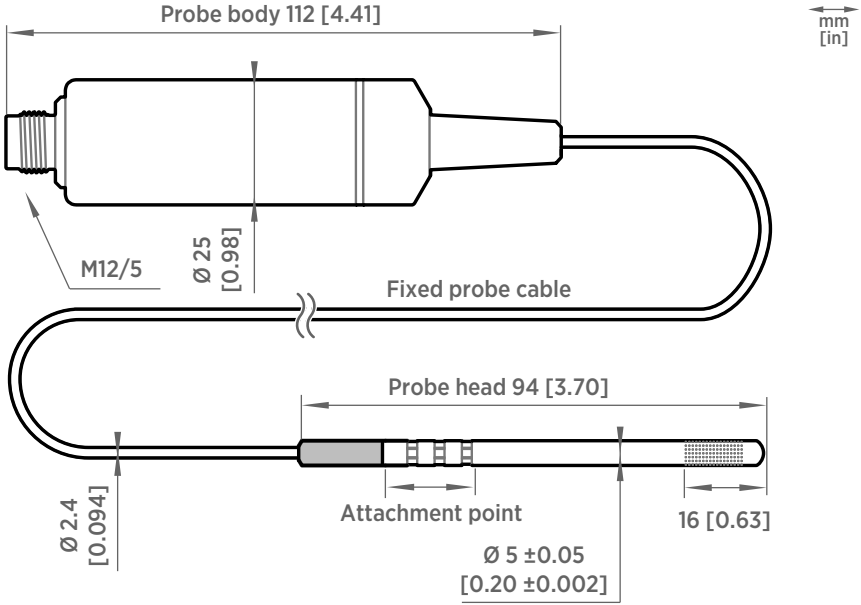


Figure 62 HMP9 probe dimensions

11.8 MMP8 specifications

Table 50 MMP8 measurement performance

| Property | Description/Value |
|---|-----------------------------------|
| Water activity | |
| Measurement range | 0-1 a _w |
| T ₉₀ response time ¹⁾ | 10 min |
| Sensor | HUMICAP® 180L2 |
| Accuracy ²⁾ | ±0.01 a _w (±1 %RS) |
| Water concentration in oil | |
| Typical accuracy | 10 % of the reading |
| Temperature | |
| Measurement range | -40 ... +180 °C (-40 ... +356 °F) |

| Property | Description/Value |
|-----------------------------|-------------------|
| Accuracy at +20 °C (+68 °F) | ±0.2 °C (0.36 °F) |

- 1) At +20 °C (+68 °F) in still oil.
- 2) In range 0–0.5 a_w , including non-linearity, hysteresis, and repeatability. See accuracy graph below.

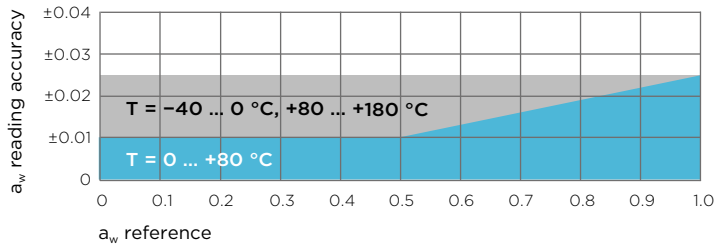
Figure 63 MMP8 A_w measurement accuracy

Table 51 MMP8 operating environment

| Property | Description/Value |
|-------------------------------------|--|
| Operating temperature of probe head | –40 ... +180 °C (–40 ... +356 °F) |
| Operating temperature of probe body | –40 ... +80 °C (–40 ... +176 °F) |
| Storage temperature range | –40 ... +80 °C (–40 ... +176 °F) |
| Operating pressure range | 0–40 bar (0–580 psi), absolute |
| Installation pressure | Up to 10 bar (145 psi), absolute |
| IP rating of probe body | IP66: Dust-tight. Protected from powerful water jets from any direction. |
| Ball valve | |
| Operating temperature | Up to +120 °C (+248 °F) |
| Operating pressure | Up to 40 bar (580 psi), absolute |

Table 52 MMP8 inputs and outputs

| Property | Description/Value |
|---------------------|----------------------|
| Operating voltage | 15–30 V DC |
| Current consumption | 10 mA typical |
| Digital output | RS-485, non-isolated |

| Property | Description/Value |
|-------------------|---|
| Protocols | Modbus RTU |
| Output parameters | Relative saturation (%RS) Temperature (°C) Water activity Water concentration in oil (ppm _w) |

Table 53 MMP8 compliance

| Property | Value/Description |
|-------------------------------------|---|
| EU directives and regulations | EMC Directive (2014/30/EU) RoHS Directive (2011/65/EU) amended by 2015/863 |
| Electromagnetic compatibility (EMC) | EN 61326-1, industrial environment |
| Compliance marks | CE, China RoHS, RCM |
| Type approvals | DNV GL certificate no. TAA00002YT ¹⁾ |

1) DNV GL certificate applies to the 262-mm-long MMP8 model only, not to the 448-mm-long model.

Table 54 MMP8 mechanical specifications

| Property | Description/Value |
|-------------------------------|---|
| Connector | M12 5-pin A-coded male |
| Weight (with a 2-m cable) | 262-mm-long MMP8: 510 g (18.0 oz) 448-mm-long MMP8: 610 g (21.5 oz) |
| Filter options | Stainless steel grid standard filter Stainless steel grid filter for high flow rates (> 1 m/s) |
| Probe cable length | 2 m (6.56 ft) |
| Adjustable installation depth | 262-mm-long MMP8: 35–193 mm (1.37–7.59 in) 448-mm-long MMP8: 35–379 mm (1.37–14.92 in) |
| Materials | |
| Probe | AISI 316L |
| Probe body | AISI 316L |
| Cable jacket | FEP |

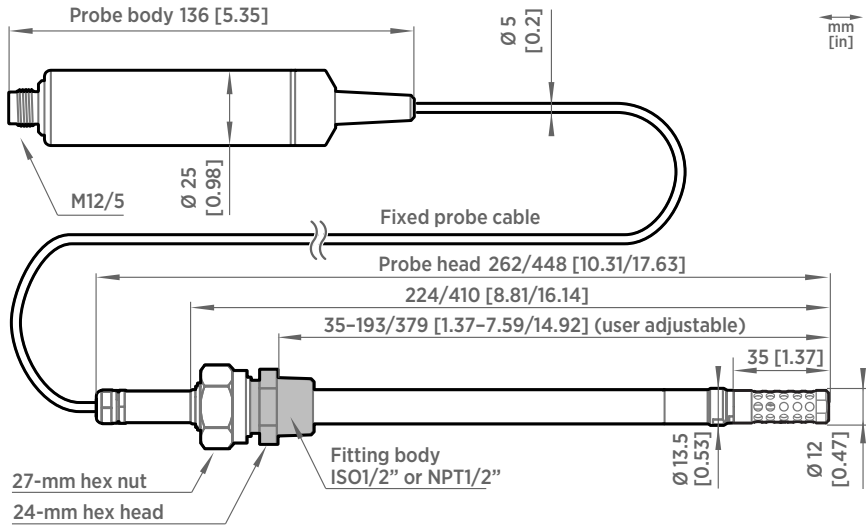


Figure 64 MMP8 dimensions

11.9 TMP1 specifications

Table 55 TMP1 measurement performance

| Property | Description/Value |
|--|---|
| Measurement range | -70 ... +180 °C (-94 ... +356 °F) |
| Sensor | Pt100 RTD Class F0.1 IEC 60751 |
| Standard calibration ^{1) 2)} | |
| Accuracy at +23 °C (+73.4 °F) | ±0.1 °C (±0.18 °F) |
| Factory calibration uncertainty ³⁾ | ±0.1 °C (±0.18 °F) at +23 °C (+73.4 °F) |
| Optional ISO 17025 calibration ^{4) 2)} | |
| Accuracy at +23 °C (+73.4 °F) ¹⁾ | ±0.06 °C (±0.108 °F) |

| Property | Description/Value |
|---------------------------------------|----------------------|
| Calibration uncertainty ³⁾ | ±0.03 °C (±0.054 °F) |

- 1) Defined against calibration reference. Including non-linearity, hysteresis, and repeatability.
- 2) Exposing temperature sensor to temperatures outside -20 ... +150 °C (-4 ... +302 °F) may cause permanent additional deviation of ±0.1 °C (0.18 °F)
- 3) Defined as ±2 standard deviation limits. Small variations possible; see calibration certificate.
- 4) Accuracy depends on selected calibration points. Accuracy with ISO 17025 calibration is defined here using a 5-point calibration in the following points: -30, -10, 0, +30, and +60 °C. For more information on calibration services offered by Vaisala, see vaisala.com/calibration.

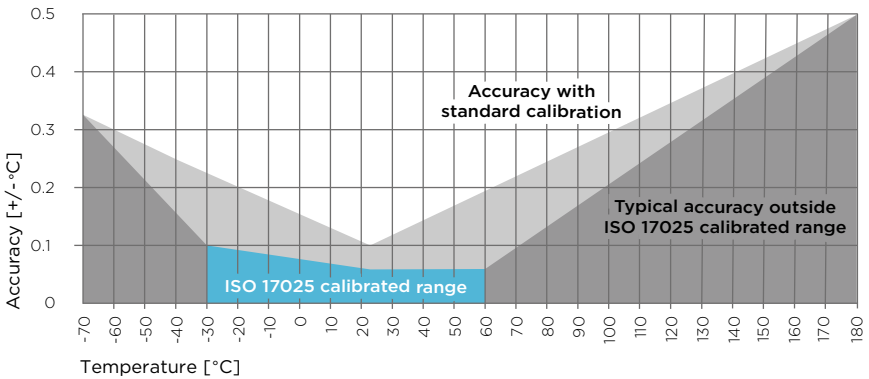


Figure 65 TMP1 temperature measurement accuracy over full range

Table 56 TMP1 operating environment

| Property | Description/Value |
|-------------------------------------|--|
| Operating temperature of probe body | -40 ... +80 °C (-40 ... +176 °F) |
| Operating temperature of probe head | -70 ... +180 °C (-94 ... +356 °F) |
| Storage temperature | -40 ... +80 °C (-40 ... +176 °F) |
| Operating environment | Suitable for outdoor use |
| IP rating | |
| Probe body | IP66: Dust-tight. Protected from powerful water jets from any direction. |

| Property | Description/Value |
|----------------------|--|
| Probe head and cable | IPX8/IPX9: Protected against high pressure and temperature water jets. Protected from the effects of continuous immersion in water. Tested under the following conditions: <ul style="list-style-type: none"> • Immersion depth: 150 cm (59 in) • Immersion time: 60 min |

Table 57 TMP1 inputs and outputs

| Property | Description/Value |
|---------------------|---|
| Operating voltage | 15–30 V DC |
| Current consumption | 10 mA typical |
| Digital output | RS-485, non-isolated |
| Protocols | Modbus RTU |
| Output parameters | Temperature (°C) Water vapor saturation pressure (hPa) |

Table 58 TMP1 compliance

| Property | Value/Description |
|-------------------------------------|---|
| EU directives and regulations | EMC Directive (2014/30/EU) RoHS Directive (2011/65/EU) amended by 2015/863 |
| Electromagnetic compatibility (EMC) | EN 61326-1, industrial environment |
| Type approvals | DNV GL certificate no. TAA00002YT |
| Compliance marks | CE, China RoHS, RCM |

Table 59 TMP1 mechanical specifications

| Property | Description/Value |
|---------------------------|---------------------------------|
| Connector | M12 5-pin A-coded male |
| Weight (with a 2-m cable) | 224 g (7.9 oz) |
| Probe cable length | 2 m (6.56 ft) or 10 m (32.8 ft) |
| Materials | |
| Probe | AISI 316L |
| Probe body | AISI 316L |

| Property | Description/Value |
|--------------|-------------------|
| Cable jacket | FEP |

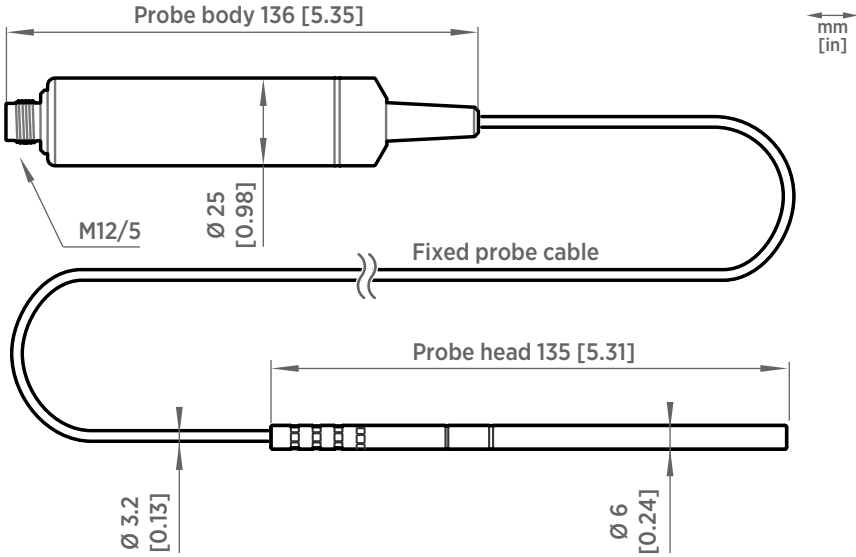


Figure 66 TMP1 probe dimensions

11.10 Accessories and spare parts



Information on spare parts, accessories, and calibration products is available online at www.vaisala.com and store.vaisala.com.

Connection cables

Table 60 Connection cables

| Description | Item code |
|---|----------------|
| Connection cable, M12-5F - M12-5M, 1 m | INDIGOCABLE1M |
| Connection cable, M12-5F - M12-5M, 3 m | INDIGOCABLE3M |
| Connection cable, M12-5F - M12-5M, 5 m | INDIGOCABLE5M |
| Connection cable, M12-5F - M12-5M, 10 m | INDIGOCABLE10M |

| Description | Item code |
|---|-----------------|
| Connection cable, M12-5F - open wires, 0.3 m | CBL210896-03MSP |
| Connection cable, M12-5F - open wires, 1 m | CBL210896-1MSP |
| Connection cable, M12-5F - open wires, 3 m | CBL210896-3MSP |
| Connection cable, M12-5F - open wires, 5 m | CBL210896-5MSP |
| Connection cable, M12-5F - open wires, 10 m | CBL210896-10MSP |
| Connection cable, M12-5F - open wires, 1.5 m | 223263SP |
| Connection cable, M12-5F - open wires, 10 m | 216546SP |
| Connection cable, M12-5F 90° - open wires, 0.6 m | 244669SP |
| Flat cable, M12-5F - M12-5M, 1 m | CBL210493SP |
| Connection cable for Indigo80, M12-5F - M12-5M, 1.5 m | 272075SP |
| Vaisala Indigo USB adapter ¹⁾ | USB2 |

1) *Vaisala Insight software for Windows available at www.vaisala.com/insight*

HMP3

Table 61 HMP3 accessories

| Description | Item code |
|---|-------------|
| Duct installation kit for humidity probe | 210697 |
| Solar radiation shield DTR502B | DTR502B |
| Cable gland M20×1.5 with split seal | HMP247CG |
| Magnetic probe holder for Ø 12 mm probe heads ¹⁾ | ASM213382SP |

1) *Not suitable for use at extreme temperatures.*

Table 62 HMP3 spare parts

| Description | Item code |
|---------------------------------|-----------|
| Sensors | |
| HUMICAP® R2 | HUMICAPR2 |
| Filters | |
| Sintered stainless steel filter | HM47280SP |

| Description | Item code |
|--|-------------|
| Stainless steel grid filter | HM47453SP |
| Metallized PPS plastic grid filter | DRW010276SP |
| Metallized PPS plastic grid with stainless steel mesh filter | DRW010281SP |

HMP4

Table 63 HMP4 spare parts

| Description | Item code |
|--|-------------|
| Sintered stainless steel filter | HM47280SP |
| Stainless steel grid | HM47453SP |
| Metallized PPS plastic grid with stainless steel mesh filter | DRW010281SP |
| Metallized PPS plastic grid filter | DRW010276SP |
| Fitting body M22×1.5 | 17223SP |
| Fitting body NPT 1/2" | 17225SP |

HMP5

Table 64 HMP5 accessories

| Description | Item code |
|-------------------------------|-----------|
| Mounting flange | 210696 |
| Calibration adapter for HMK15 | 211302SP |

Table 65 HMP5 spare parts

| Description | Item code |
|--|-------------|
| Sintered stainless steel filter | HM47280SP |
| Stainless steel grid | HM47453SP |
| Metallized PPS plastic grid with stainless steel mesh filter | DRW010281SP |
| Metallized PPS plastic grid filter | DRW010276SP |

HMP7

Table 66 HMP7 accessories

| Description | Item code |
|---|-------------|
| Duct installation kit for humidity probe | 210697 |
| Solar radiation shield DTR502B | DTR502B |
| Warmed probe accessory | HMT330WPA |
| Cable gland M20×1.5 with split seal | HMP247CG |
| Swagelok® for 12 mm probe, 1/2" ISO thread | SWG12ISO12 |
| Swagelok® for 12 mm probe, 3/8" ISO thread | SWG12ISO38 |
| Swagelok® for 12 mm probe, 1/2" NPT thread | SWG12NPT12 |
| Magnetic probe holder for Ø 12 mm probe heads 1) | ASM213382SP |
| Calibration adapter for HMK15 | 211302SP |

1) Not suitable for use at extreme temperatures.

Table 67 HMP7 spare parts

| Description | Item code |
|--|-------------|
| Sintered stainless steel filter | HM47280SP |
| Stainless steel grid | HM47453SP |
| Metallized PPS plastic grid with stainless steel mesh filter | DRW010281SP |
| Metallized PPS plastic grid filter | DRW010276SP |
| Membrane stainless steel filter for fuel cell applications | 214848SP |

HMP8

Table 68 HMP8 accessories

| Description | Item code |
|--|-------------|
| Ball valve kit ISO 1/2" with welding joint | BALLVALVE-1 |
| Calibration adapter for HMK15 | 211302SP |

| Description | Item code |
|--|-----------|
| Weatherproof carrying case for Indigo80 and a series 8 probe ¹⁾ | ASM215318 |

1) For example, MMP8, HMP8, or DMP8 with a max. 2-m (6.6-ft) probe connection cable.

Table 69 HMP8 spare parts

| Description | Item code |
|--|-------------|
| Sintered stainless steel filter | HM47280SP |
| Stainless steel grid | HM47453SP |
| Metallized PPS plastic grid with stainless steel mesh filter | DRW010281SP |
| Metallized PPS plastic grid filter | DRW010276SP |
| Fitting body NPT 1/2" | 212810SP |
| Fitting body ISO R 1/2" | DRW212076SP |
| Thread adapter ISO 1/2" to NPT 1/2" | 210662SP |
| Manual pressing handle | HM36854SP |

HMP9

Table 70 HMP9 accessories

| Description | Item code(s) |
|--|--------------------|
| HMP9 calibration adapter for HMK15 | ASM213801 |
| HMP9 duct installation kit | ASM214055 |
| Solar radiation shield DTR502B with sensor head support 215130 | DTR502B and 215130 |

Table 71 HMP9 spare parts

| Description | Item code(s) |
|-------------|--------------|
| Gland set | ASM213199 |

MMP8

Table 72 MMP8 accessories

| Description | Item code |
|--|-------------|
| Ball valve kit ISO 1/2" with welding joint | BALLVALVE-1 |
| Ball valve kit ISO 1/2" – ISO 3/4" with thread joint | BALLVALVE-2 |
| Calibration adapter for HMK15 | 211302SP |
| Weatherproof carrying case for Indigo80 and a series 8 probe ¹⁾ | ASM215318 |

1) For example, MMP8, HMP8, or DMP8 with a max. 2-m (6.6-ft) probe connection cable.

Table 73 MMP8 spare parts

| Description | Item code |
|---|-------------|
| Stainless steel grid filter | HM47453SP |
| Stainless steel grid filter for high flow rates (> 1 m/s) | 220752SP |
| Fitting body NPT 1/2" | 212810SP |
| Fitting body ISO R 1/2" | DRW212076SP |
| Manual pressing handle | HM36854SP |

TMP1

Table 74 TMP1 accessories

| Description | Item code |
|---|-----------|
| Duct installation kit for temperature probe | 215003 |
| Swagelok® for 6 mm probe, 1/8" ISO thread | SWG6ISO18 |
| Swagelok® for 6 mm probe, 1/8" NPT thread | SWG6NPT18 |

11.11 Accuracy of calculated output parameters

HMP series probes measure relative humidity and temperature, and calculate the other output parameters from those two parameters. Accuracy of the calculated parameters is derived from the accuracy of the original RH and T measurements.

Use the Vaisala Humidity Calculator to convert the accuracy specification of RH measurement for other humidity parameters. You can download it from www.vaisala.com.

VAISALA Humidity Calculator Help Units Theme English

Basic **Advanced** Reset

Ambient conditions

Temperature: °C
 Pressure: hPa
 Gas:

Select known humidity parameter

| | From | → | To |
|---------------------------|--|---|--------------------------------|
| Relative humidity | <input type="text" value="50"/> ± <input type="text" value="1"/> %rh | | 50.0000 ± 1.0 %rh |
| Dew/frost point temp. | | | 12.0323 ± 0.3 °C |
| Absolute humidity | | | 10.3250 ± 0.2 g/m ³ |
| Mixing ratio | | | 8.78510 ± 0.2 g/kg |
| Wet-bulb temperature | | | 16.3422 ± 0.2 °C |
| Enthalpy | | | 45.4813 ± 0.5 kJ/kg |
| Rel. humidity (dew/frost) | | | 50.0000 ± 1.0 %rh |
| Dew point temperature | | | 12.0323 ± 0.3 °C |
| Water concentration | | | 14124.3 ± 287 ppm _v |
| Water conc. (wet basis) | | | 13927.6 ± 279 ppm _v |
| Water vapor pressure | | | 14.1121 ± 0.3 hPa |
| Water vapor satur. press. | | | 28.2243 hPa |

Figure 67 Vaisala Humidity Calculator in Advanced mode

Appendix A. Modbus reference

A.1 Default communication settings

Table 75 Default Modbus serial communication settings

| Property | Description/Value |
|-----------------------|-------------------|
| Serial bit rate | 19200 |
| Parity | None |
| Number of data bits | 8 |
| Number of stop bits | 2 |
| Flow control | None |
| Modbus device address | 240 |

You can use up to ten probes on the same RS-485 line. You must configure each probe on the line to have a different Modbus address.

A.2 Function codes

Table 76 Modbus function codes

| Function code (decimal) | Function code (hexadecimal) | Name | Notes |
|-------------------------|---------------------------------------|----------------------------|---------|
| 03 | 03 _{hex} | Read Holding Registers | Class 0 |
| 16 | 10 _{hex} | Write Multiple Registers | Class 0 |
| 43 / 14 | 2B _{hex} / 0E _{hex} | Read Device Identification | |

A.3 Data encoding

In the data registers, the numeric values are available in one or two formats with separate register addresses: 32-bit IEEE floating point format and/or 16-bit signed integer format.



For values that have both 32-bit and 16-bit register available, use of the 32-bit register is recommended. Some values may exceed the signed 16-bit range even in normal operation.

A.3.1 32-bit floating point or 32-bit integer format

Registers using **32-bit float** data format are encoded using the **binary32** encoding defined in IEEE 754. The format is also known as "single-precision floating point format".

The least significant 16 bits of a floating point number are placed at the Modbus register listed in the table, while the most significant 16 bits are placed in the register with number/address + 1, as specified in Open Modbus TCP Specification, Release 1.0. This is also known as "little-endian" or "Modicon" word order.

Despite the specification, some Modbus masters may expect a "big-endian" word order (most significant word first). In such case, you must select "word-swapped" floating point format in your Modbus master for the Modbus registers of the device.

A complete 32-bit floating point or 32-bit integer value should be read and written in a single Modbus transaction.



CAUTION! Reading the measurement data registers with incorrect floating point format setting may occasionally result in correct-looking, but nevertheless incorrect values.



It is highly recommended to verify that you have configured the floating point format correctly on your Modbus host system by reading a floating point value from a test value register.

A.3.2 16-bit integer format

Some 16-bit integer values in the data registers are scaled to include the necessary decimals. The scaling factors for those values are shown in the register tables.

Table 77 Interpretation of 16-bit signed integer values

| Value (decimal) | Value (hexadecimal) | Description |
|-----------------|---------------------|---|
| 0–32766 | 0x0000–0x7FFE | Value in range 0–32766 |
| 32767 | 0x7FFF | Value is 32767 or larger |
| 32768 | 0x8000 | Value is not available |
| 32769 | 0x8001 | Value is –32767 or smaller |
| 32770–65535 | 0x8002–0xFFFF | Value in range –32766 ... –1 (2's complement) |

A.4 Modbus registers

Registers are numbered in decimal, starting from 1. Register addresses in actual Modbus messages (Modbus Protocol Data Unit (PDU)) are in hexadecimal and start from zero. Register number 1 corresponds to address 0x0 in the actual Modbus message.



CAUTION! Reading the wrong register(s) may result in correct-looking values. Check the reference documentation of your Modbus host (PLC) to verify which notation it uses for Modbus register addresses.

A.4.1 Measurement data registers

Table 78 Floating point measurement data registers (read-only)

| Register number | Address | Description | Data format | Unit |
|-----------------|---------------------|--------------------------------------|--------------|------------------|
| 1 | 0000 _{hex} | Relative humidity | 32-bit float | %RH |
| 3 | 0002 _{hex} | Temperature | 32-bit float | °C |
| 7 | 0006 _{hex} | Dew point temperature | 32-bit float | °C |
| 9 | 0008 _{hex} | Dew/frost point temperature | 32-bit float | °C |
| 11 | 000A _{hex} | Dew/frost point temperature at 1 atm | 32-bit float | °C |
| 13 | 000C _{hex} | Dew point temperature at 1 atm | 32-bit float | °C |
| 15 | 000E _{hex} | Absolute humidity | 32-bit float | g/m ³ |
| 17 | 0010 _{hex} | Mixing ratio | 32-bit float | g/kg |
| 19 | 0012 _{hex} | Wet-bulb temperature | 32-bit float | °C |
| 21 | 0014 _{hex} | Water concentration | 32-bit float | ppm _v |
| 23 | 0016 _{hex} | Water vapor pressure | 32-bit float | hPa |
| 25 | 0018 _{hex} | Water vapor saturation pressure | 32-bit float | hPa |
| 27 | 001A _{hex} | Enthalpy | 32-bit float | kJ/kg |
| 29 | 001C _{hex} | Water activity | 32-bit float | |
| 31 | 001E _{hex} | Dew point temperature difference | 32-bit float | °C |
| 33 | 0020 _{hex} | Absolute humidity at NTP | 32-bit float | g/m ³ |
| 35 | 0022 _{hex} | Water concentration in oil | 32-bit float | ppm _w |
| 41 | 0028 _{hex} | Relative saturation | 32-bit float | %RS |
| 43 | 002A _{hex} | Water concentration (wet basis) | 32-bit float | vol-% |

| Register number | Address | Description | Data format | Unit |
|-----------------|---------------------|-------------------------------|--------------|------------------|
| 45 | 002C _{hex} | Relative humidity (dew/frost) | 32-bit float | %RH |
| 65 | 0040 _{hex} | Water mass fraction | 32-bit float | ppm _w |

Table 79 Integer measurement data registers (read-only)

| Register number | Address | Description | Data format | Scale factor | Offset | Unit |
|-----------------|---------------------|--------------------------------------|-----------------------|--------------|--------|------------------|
| 257 | 0100 _{hex} | Relative humidity | 16-bit signed integer | 100 | 0 | %RH |
| 258 | 0101 _{hex} | Temperature | 16-bit signed integer | 100 | 0 | °C |
| 260 | 0103 _{hex} | Dew point temperature | 16-bit signed integer | 100 | 0 | °C |
| 261 | 0104 _{hex} | Dew/frost point temperature | 16-bit signed integer | 100 | 0 | °C |
| 262 | 0105 _{hex} | Dew/frost point temperature at 1 atm | 16-bit signed integer | 100 | 0 | °C |
| 263 | 0106 _{hex} | Dew point temperature at 1 atm | 16-bit signed integer | 100 | 0 | °C |
| 264 | 0107 _{hex} | Absolute humidity | 16-bit signed integer | 100 | 0 | g/m ³ |
| 265 | 0108 _{hex} | Mixing ratio | 16-bit signed integer | 100 | 0 | g/kg |
| 266 | 0109 _{hex} | Wet-bulb temperature | 16-bit signed integer | 100 | 0 | °C |
| 267 | 010A _{hex} | Water concentration | 16-bit signed integer | 1 | 0 | ppm _v |
| 268 | 010B _{hex} | Water vapor pressure | 16-bit signed integer | 10 | 0 | hPa |
| 269 | 010C _{hex} | Water vapor saturation pressure | 16-bit signed integer | 10 | 0 | hPa |
| 270 | 010D _{hex} | Enthalpy | 16-bit signed integer | 100 | 0 | kJ/kg |
| 271 | 010E _{hex} | Water activity | 16-bit signed integer | 10000 | 0 | - |

| Register number | Address | Description | Data format | Scale factor | Offset | Unit |
|-----------------|---------------------|----------------------------------|-----------------------|--------------|--------|------------------|
| 272 | 010F _{hex} | Dew point temperature difference | 16-bit signed integer | 10 | 0 | °C |
| 273 | 0110 _{hex} | Absolute humidity at NTP | 16-bit signed integer | 100 | 0 | g/m ³ |
| 274 | 0111 _{hex} | Water concentration in oil | 16-bit signed integer | 1 | 0 | ppm _w |
| 277 | 0114 _{hex} | Relative saturation | 16-bit signed integer | 100 | 0 | %RS |
| 278 | 0115 _{hex} | Water concentration (wet basis) | 16-bit signed integer | 100 | 0 | vol-% |
| 279 | 0116 _{hex} | Relative humidity (dew/frost) | 16-bit signed integer | 100 | 0 | %RH |
| 289 | 0120 _{hex} | Water vapor mass fraction | 16-bit signed integer | 1 | 0 | ppm _w |

A.4.2 Configuration registers

Table 80 Modbus configuration data registers (writable)

| Register number | Address | Description | Data format | Unit/Valid range |
|-----------------|---------------------|--|----------------|--|
| General | | | | |
| 1287 | 0506 _{hex} | <p>Condensation prevention on/off. Enables the condensation prevention heating functions of the device.</p> <p>When warming is active, values of output parameters that depend on temperature measurement (for example, relative humidity) are unavailable unless temperature is written to register 0334_{hex} from an external source.</p> | 16-bit boolean | <p>0 = off (default)</p> <p>1 = on</p> |

| Compensation setpoints | | | | |
|-------------------------------|---------------------|--|----------------|--|
| 769 | 0300 _{hex} | <p>Pressure compensation setpoint</p> <p>The entered value is persistent and remains unchanged at device restart.</p> | 32-bit float | <p>Unit: hPa</p> <p>Default: 1013.25 hPa</p> |
| 821 | 0334 _{hex} | <p>Temperature compensation setpoint. If a value is written to this register, probe uses it instead of its own temperature measurement.</p> <p>When condensation prevention warming is active, temperature must be written to this register to enable output parameters that depend on temperature measurement (for example, relative humidity).</p> <p>At device reset, the value is cleared.</p> | 32-bit float | Unit: °C |
| Sensor purge | | | | |
| 773 | 0304 _{hex} | Sensor purge interval | 32-bit float | Unit: min 10 ... 14400 |
| 1283 | 0502 _{hex} | Interval purge on/off | 16-bit boolean | 0 = Off 1 = On |
| 1284 | 0503 _{hex} | Startup purge on/off | 16-bit boolean | 0 = Off 1 = On |

| Filtering | | | | |
|----------------------|---------------------|---|----------------|---|
| 795 | 031A _{hex} | Measurement filtering factor | 32-bit float | Range: 0.000 ... 1.000 1.000 = Reading shows 100% of the most recent measured value (no filtering, default) 0.01 ... 0.99 = Reading shows 1 ... 99% of the most recent measured value and part of the previous reading (filtering is applied). For example, "0.9" means that the filtered measurement reading = 90% of the most recent measured value + 10% of the previous reading. |
| 1282 | 0501 _{hex} | Enable of disable measurement filtering using the user-defined filtering factor (register 031A _{hex}) | 16-bit boolean | 0 = Off 1 = On |
| Communication | | | | |
| 1537 | 0600 _{hex} | Modbus address | 16-bit integer | 1 ... 247 Default: 240 |
| 1538 | 0601 _{hex} | Bit rate | enum | 0 = 300 1 = 600 2 = 1200 3 = 2400 4 = 4800 5 = 9600 6 = 19200 7 = 38400 8 = 57600 9 = 115200 |

| Communication | | | | |
|---------------|---------------------|-------------------------|----------------|---|
| 1539 | 0602 _{hex} | Parity, data, stop bits | enum | 0 = None, 8, 1 1 = None, 8, 2 2 = Even, 8, 1 3 = Even, 8, 2 4 = Odd, 8, 1 5 = Odd, 8, 2 (default: 1 = None, 8, 2) |
| 1540 | 0603 _{hex} | Response delay | 16-bit integer | Unit: ms Range: 0 ... 1000 |

Table 81 Modbus function registers (writable)

| Register number | Address | Description | Data format | Unit/Valid range |
|------------------|---------------------|--------------------|----------------|--|
| Functions | | | | |
| 1285 | 0504 _{hex} | Start sensor purge | 16-bit integer | When writing to register: 1 = Start sensor purge When sensor purge is in progress, the value of the register will count up from 0 to 100. When the value reaches 100 the sensor purge is complete. |
| 1542 | 0605 _{hex} | Restart device | 16-bit integer | When writing to register: 1 = Restart the device |

A.4.3 Status registers

Table 82 Modbus status data registers (read-only)

| Register number | Address | Description | Data format | Note |
|-----------------|---------------------|--------------|----------------|--|
| 513 | 0200 _{hex} | Error status | 16-bit boolean | 0000_{hex} : One or more errors active 0001_{hex} : No errors |

| Register number | Address | Description | Data format | Note |
|-----------------|---------------------|-------------------------------------|-----------------------|--|
| 514 | 0201 _{hex} | Online status | 16-bit boolean | 0000 _{hex} : Output locked 0001 _{hex} : Online data available |
| 516 | 0203 _{hex} | Error code | 32-bit signed integer | See Table 83 (page 139) . |
| 518 | 0205 _{hex} | Security hash | 32-bit signed integer | Security hash changes when any change is made to device settings or adjustments. |
| 520 | 0207 _{hex} | RH measurement status | 16-bit signed integer | 0000 _{hex} : Status OK 0001 _{hex} : Measurement is not available |
| 521 | 0208 _{hex} | T measurement status | 16-bit signed integer | 0002 _{hex} : Measurement is not reliable |
| 522 | 0209 _{hex} | T _{d/f} measurement status | 16-bit signed integer | 0004 _{hex} : Under range 0008 _{hex} : Over range 0020 _{hex} : Value locked 0080 _{hex} : Sensor failure 0100 _{hex} : Measurement is not ready |
| 523 | 020A _{hex} | Device status | 16-bit signed integer | 0000 _{hex} : Status OK 0001 _{hex} : Critical error, maintenance needed 0002 _{hex} : Error, device may recover automatically 0004 _{hex} : Warning 0008 _{hex} : Notification 0010 _{hex} : Calibration mode active |

Table 83 Error codes in register 0203_{hex}

| Bitmask | Error message | Severity |
|---------------------|-------------------------------|----------|
| 0000 _{hex} | Status OK | |
| 0001 _{hex} | Temperature measurement error | Error |
| 0002 _{hex} | Humidity measurement error | Error |

| Bitmask | Error message | Severity |
|-----------------------|----------------------------------|----------|
| 0004 _{hex} | Humidity sensor failure | Error |
| 0008 _{hex} | Capacitance reference error | Error |
| 0010 _{hex} | Ambient temperature out of range | Error |
| 800000 _{hex} | Sensor heater failure | Warning |

A.4.4 Test value registers

Read the known test values from the test registers to verify the functionality of your Modbus implementation.

Table 84 Modbus test registers (read-only)

| Register number | Address | Description | Data format | Test value |
|-----------------|---------------------|----------------|--------------------------|-----------------------|
| 7937 | 1F00 _{hex} | Signed integer | 16-bit integer | -12345 |
| 7938 | 1F01 _{hex} | Floating point | 32-bit float | -123.45 |
| 7940 | 1F03 _{hex} | Text string | 7-character ASCII string | Text string "-123.45" |

A.5 Device identification objects

Table 85 Device identification objects

| Object ID | Object ID (hexadecimal) | Object name | Example contents |
|-----------|-------------------------|---------------------|---|
| 0 | 0x00 | VendorName | "Vaisala" |
| 1 | 0x01 | ProductCode | "HMP4" |
| 2 | 0x02 | MajorMinorVersion | "1.2.3" Software version of the device. |
| 3 | 0x03 | VendorUrl | " http://www.vaisala.com/ " |
| 4 | 0x04 | ProductName | "Humidity and Temperature Probe HMP4" |
| 5 | 0x05 | ModelName | "7E2A2A0A000" Configuration code of the device. Length and content of the code are model-specific. |
| 6 | 0x06 | UserApplicationName | User definable information text (see configuration register 0x0A00) |

| Object ID | Object ID (hexadecimal) | Object name | Example contents |
|-----------|-------------------------|-------------------------------|---|
| 128 | 0x80 | SerialNumber ¹⁾ | "K0710040" |
| 129 | 0x81 | CalibrationDate ¹⁾ | "2020-01-31" Calibration date in YYYY-MM-DD format. Empty string if not set/valid. |
| 130 | 0x82 | CalibrationText ¹⁾ | "Vaisala/HEL" Calibration information text. Empty string if not set/valid. |

¹⁾ *Vaisala-specific device information.*

A.6 Exception responses

Table 86 Modbus exception responses

| Code | Name | Reason |
|------|----------------------|---|
| 01 | ILLEGAL FUNCTION | Unsupported function code |
| 02 | ILLEGAL DATA ADDRESS | Register address or Object ID out of valid ranges |
| 03 | ILLEGAL DATA VALUE | Otherwise invalid request |

Accessing unavailable (temporarily missing) measurement data does not generate a Modbus exception. "Unavailable" value (a quiet NaN for floating point data or 0x8000 for integer data) is returned instead. An exception is generated only for any access outside the applicable register ranges.

A.7 Modbus communication examples

Reading relative humidity value




Device address used in the following examples is 240 (F0_{hex}).
 Measurement values returned by the device change depending on ambient conditions and/or device settings.

| Request | | Response | |
|---------------------------------|--|---------------------------------|--|
| Bytes on the line (hexadecimal) | Description | Bytes on the line (hexadecimal) | Description |
| (silence for 3.5 bytes) | Start of Modbus RTU frame | (silence for 3.5 bytes) | Start of Modbus RTU frame |
| F0 _{hex} | Probe address | F0 _{hex} | Probe address |
| 03 _{hex} | Function (Read Holding Registers) | 03 _{hex} | Function (Read Holding Registers) |
| 00 _{hex} | Register address | 04 _{hex} | Number of data bytes |
| 00 _{hex} | | 7A _{hex} | Value of first register (least significant word) |
| 00 _{hex} | Number of 16-bit registers to read (2) | E1 _{hex} | |
| 02 _{hex} | | 41 _{hex} | Value of second register (most significant word) |
| D1 _{hex} | Modbus RTU checksum | F4 _{hex} | Modbus RTU checksum |
| 2A _{hex} | | | |
| (silence for 3.5 bytes) | End of Modbus RTU frame | 05 _{hex} | |
| | | (silence for 3.5 bytes) | End of Modbus RTU frame |

| Communication description | |
|---------------------------|--|
| Register address | 1 (1-based Modbus documentation format) = 0000 _{hex} (0-based format used in actual communication). |
| Data format | Two 16-bit Modbus registers interpreted as IEEE 754 binary32 floating point value, least significant word first. |
| Returned value | 41F47AE1 _{hex} , which is binary32 representation of 30.56 (%RH). |

Writing pressure compensation value

| Request | | Response | |
|---------------------------------|--|---|--|
| Bytes on the line (hexadecimal) | Description | Bytes on the line (hexadecimal) | Description |
| (silence for 3.5 bytes) | Start of Modbus RTU frame | (silence for 3.5 bytes) | Start of Modbus RTU frame |
| F0 _{hex} | Probe address | F0 _{hex} | Probe address |
| 10 _{hex} | Function (Write Multiple Registers) | 10 _{hex} | Function (Write Multiple Registers) |
| 03 _{hex} | Register address | 03 _{hex} | Register address |
| 00 _{hex} | | 00 _{hex} | |
| 00 _{hex} | Number of registers to write (2) | 00 _{hex} | Number of 16-bit registers written (2) |
| 02 _{hex} | | 02 _{hex} | |
| 04 _{hex} | Number of data bytes | 54 _{hex} | Modbus RTU checksum |
| 6E _{hex} | Value for first register (least significant word) | AD _{hex} | |
| 14 _{hex} | | | |
| 44 _{hex} | Value for second register (least significant word) | (silence for 3.5 bytes) | End of Modbus RTU frame |
| 75 _{hex} | | | |
| 4E _{hex} | Modbus RTU checksum | <div style="border: 1px solid gray; padding: 10px;">  <p>The response to a write function informs that the function was correctly received by the device. It does not guarantee that the written value was accepted by the device (for example, in case out-of-range values).</p> <p>To verify that the value was really accepted by the device, read the register value after writing.</p> </div> | |
| AB _{hex} | | | |
| (silence for 3.5 bytes) | End of Modbus RTU frame | | |

| Communication description | |
|---------------------------|--|
| Register address | 769 (1-based Modbus documentation format) = 0300 _{hex} (0-based format used in actual communication). |

| Communication description | |
|---------------------------|--|
| Data format | Two 16-bit Modbus registers interpreted as IEEE 754 binary32 floating point value, least significant word first. |
| Value to write | 44756E14 _{hex} = 981.72 (hPa) |

Maintenance and calibration services



Vaisala offers comprehensive customer care throughout the life cycle of our measurement instruments and systems. Our factory services are provided worldwide with fast deliveries. For more information, see www.vaisala.com/calibration.

- Vaisala Online Store at store.vaisala.com is available for most countries. You can browse the offering by product model and order the right accessories, spare parts, or maintenance and calibration services.
- To contact your local maintenance and calibration expert, see www.vaisala.com/contactus.

Warranty

For standard warranty terms and conditions, see www.vaisala.com/warranty.

Please observe that any such warranty may not be valid in case of damage due to normal wear and tear, exceptional operating conditions, negligent handling or installation, or unauthorized modifications. Please see the applicable supply contract or Conditions of Sale for details of the warranty for each product.

Technical support



Contact Vaisala technical support at helpdesk@vaisala.com. Provide at least the following supporting information as applicable:

- Product name, model, and serial number
- Software/Firmware version
- Name and location of the installation site
- Name and contact information of a technical person who can provide further information on the problem

For more information, see www.vaisala.com/support.

Recycling



Recycle all applicable material according to local regulations.

VAISALA

www.vaisala.com

